


PRODUCT CATALOGUE

Biomimetic **ICEBERG**

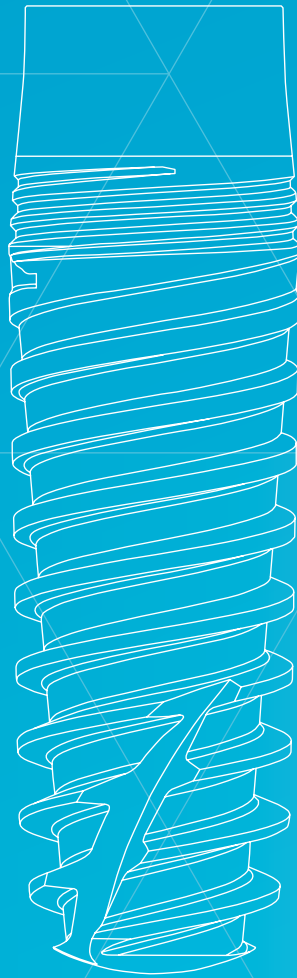


The **ICEBERG** system is a new line that adds to the range of Avinent implants and that is especially aimed at simplifying post-surgery treatments and increasing the creation of soft tissue around the implant thanks to its polished neck at a tissue level. The ICEBERG system offers a very simple and logical surgical procedure, with its own surgical kit and a simple and practical drilling protocol thanks to its color code.

CONTENTS




Surgical phase	4
CCI Iceberg Connection	4
Accessories	6
Drill Stops	8
Instruments and surgical kit	10
Drilling speed	11
Drill-bit length and marking	11
Accessories CC.I	11
Platform indicators	11
Avinent drilling biological protocol	12
Avinent drilling standard protocol	14
Sterilization and packaging	16
Avinent Guided Surgery	18
Micromotors	18
Radiographic template	18
Product index	19

Biomimetic ICEBERG











ICEBERG CONNECTION

















SURGICAL PHASE



	Platform Ø 3,5 mm				
	Ø 3,5 mm	Ref.	Ø 4,0 mm	Ref.	Ø 4,5 mm
Implant 	- - 3,5 x 10 mm 3,5 x 11,5 mm 3,5 x 13 mm 3,5 x 15 mm	- - 5900 5901 5902 5903	4,0 x 7 mm 4,0 x 8,5 mm 4,0 x 10 mm 4,0 x 11,5 mm 4,0 x 13 mm 4,0 x 15 mm	5904 5905 5906 5907 5908 5909	4,5 x 7 mm 4,5 x 8,5 mm 4,5 x 10 mm 4,5 x 11,5 mm 4,5 x 13 mm 4,5 x 15 mm
Healing abutment 	3,5 x 2 mm 3,5 x 3 mm 3,5 x 5 mm	5922 5923 5924	3,5 x 2 mm 3,5 x 3 mm 3,5 x 5 mm	5922 5923 5924	3,5 x 2 mm 3,5 x 3 mm 3,5 x 5 mm
Anatomic healing abutment 	4 x 2 mm 4 x 3 mm 4 x 5 mm 5 x 2 mm 5 x 3 mm 5 x 5 mm	5928 5929 5930 5931 5932 5933	4 x 2 mm 4 x 3 mm 4 x 5 mm 5 x 2 mm 5 x 3 mm 5 x 5 mm	5928 5929 5930 5931 5932 5933	4 x 2 mm 4 x 3 mm 4 x 5 mm 5 x 2 mm 5 x 3 mm 5 x 5 mm









			Platform Ø 4,1 mm			
Ref.	Ø 5,0 mm	Ref.	Ø 4,5 mm	Ref.	Ø 5,0 mm	Ref.
6309	5,0 x 7 mm	6315	4,5 x 7 mm	5910	5,0 x 7 mm	5917
6310	5,0 x 8,5 mm	6316	4,5 x 8,5 mm	5911	5,0 x 8,5 mm	5918
6311	5,0 x 10 mm	6317	4,5 x 10 mm	5912	5,0 x 10 mm	5919
6312	5,0 x 11,5 mm	6318	4,5 x 11,5 mm	5913	5,0 x 11,5 mm	5920
6313	-	-	4,5 x 13 mm	5914	-	-
6314	-	-	4,5 x 15 mm	5915	-	-
5922	3,5 x 2 mm	5922	4 x 2 mm	5925	4 x 2 mm	5925
5923	3,5 x 3 mm	5923	4 x 3 mm	5926	4 x 3 mm	5926
5924	3,5 x 5 mm	5924	4 x 5 mm	5927	4 x 5 mm	5927
5928	4 x 2 mm	5928	5 x 2 mm	5934	5 x 2 mm	5934
5929	4 x 3 mm	5929	5 x 3 mm	5935	5 x 3 mm	5935
5930	4 x 5 mm	5930	5 x 5 mm	5936	5 x 5 mm	5936
5931	5 x 2 mm	5931	6 x 2 mm	5937	6 x 2 mm	5937
5932	5 x 3 mm	5932	6 x 3 mm	5938	6 x 3 mm	5938
5933	5 x 5 mm	5933	6 x 5 mm	5939	6 x 5 mm	5939

ACCESSORIES

		Ref.
Sterilization cassette Ocean		1763
MiniBox		0526
Torque wrench		0295
Screwdrivers		
	Screwdriver ISO 1797 S (048)	0644
	Screwdriver ISO 1797 L (048)	0277
	Screwdriver ISO 1797 XL (048)	0645
	Implant driver ISO 1797 EC/IC S (2.5)	2693
	Implant driver ISO 1797 EC/IC L (2.5)	0300
	Implant driver ISO 1797 W&H EC/IC (2.5)	2692
	Screwdriver gold screw ISO 1797	0263
	Screwdriver Rhein 83 abutment	
	Screwdriver grooved screw ISO 1797	0267
	Screwdriver impression coping closed tray ISO 1797	0723
	Screwdriver transepithelial abutment ISO 1797 S	0328
	Screwdriver transepithelial abutment ISO 1797 L	0726
	Screwdriver transepithelial angled abutment ISO 1797 S	0804
	Screwdriver transepithelial angled abutment ISO 1797 L	0648
	Implant driver ISO 1797 CC 3,5 S	2981
	Implant driver ISO 1797 CC 3,5 L	2984
	Implant driver ISO 1797 CC 4,1 S	2982
	Implant driver ISO 1797 CC 4,1 L	2985


Screwdriver handle		Handle ISO 1797 S		0791
		Handle ISO 1797 L		0790
Implant handle	<input type="checkbox"/> 	Implant handle S		1878
	<input type="checkbox"/> 	Implant handle L		2891
Monoblock screwdrivers		Screwdriver S (048)		0274
		Screwdriver L (048)		0275
	<input type="checkbox"/> 	Implant driver S (2.5)		0278
	<input type="checkbox"/> 	Implant driver L (2.5)		0299
Drills		Pointed drill		0188
		Twist drill	1,6 x 7 - 15 mm	2046
		Pilot drill	1,6 - 2,4 mm	2047
		Drill	2,0 - 3,3 x 7 - 15 mm 2,2 - 3,8 x 7 - 15 mm 2,8 - 4,3 x 7 - 15 mm 3,2 - 4,8 x 7 - 13 mm	2048 2049 2050 2051
		Hard bone drill	2,4 - 3,3 x 7 - 15 mm 3,0 - 3,7 x 7 - 15 mm 3,8 - 4,3 x 7 - 15 mm 4,1 - 4,7 x 7 - 13 mm	3311 3312 3313 3314
			2,0 - 3,3 x 7 - 15 mm 2,2 - 3,8 x 7 - 15 mm 2,8 - 4,3 x 7 - 15 mm 3,2 - 4,8 x 7 - 13 mm 4,2 - 5,7 x 7 - 11,5 mm	8032 8033 8034 8035 8036
			2,4 - 3,3 x 7 - 15 mm 3,0 - 3,7 x 7 - 15 mm 3,8 - 4,3 x 7 - 15 mm 4,1 - 4,7 x 7 - 13 mm 5,1 - 5,7 x 7 - 11,5 mm	8037 8038 8039 8040 8041
Screw tap		Screw tap	3,5 mm 4,0 mm 4,5 mm 5,0 mm	2687 2688 2689 2690

Direction indicator		1,5 - 2,3 mm	1810
Drill extension ISO 1797			KI589B204

Drill stops		Ø1,3-2,4 L7	6984
		Ø1,3-2,4 L8,5	6985
		Ø1,3-2,4 L10	6986
		Ø1,3-2,4 L11,5	6987
		Ø1,3-2,4 L13	6988
		Ø1,3-2,4 L15	6989
			Ø2,8-3,3 L7
Ø2,8-3,3 L8,5	6991		
Ø2,8-3,3 L10	6992		
Ø2,8-3,3 L11,5	6993		
Ø2,8-3,3 L13	6994		
Ø2,8-3,3 L15	6995		
	Ø3,2-3,8 L7	6996	
	Ø3,2-3,8 L8,5	6997	
	Ø3,2-3,8 L10	6998	
	Ø3,2-3,8 L11,5	6999	
	Ø3,2-3,8 L13	7000	
	Ø3,2-3,8 L15	7001	
	Ø3,6-4,3 L7	7002	
	Ø3,6-4,3 L8,5	7003	
	Ø3,6-4,3 L10	7004	
	Ø3,6-4,3 L11,5	7005	
	Ø3,6-4,3 L13	7006	
	Ø3,6-4,3 L15	7007	
	Ø4,2-4,8 L7	7008	
	Ø4,2-4,8 L8,5	7009	
	Ø4,2-4,8 L10	7010	
	Ø4,2-4,8 L11,5	7011	
	Ø4,2-4,8 L13	7012	
	Ø5,7 L7	7013	
	Ø5,7 L8,5	7014	
	Ø5,7 L10	7015	
	Ø5,7 L11,5	7016	
Drill Stops Kit for implants up to Ø4,5			7959
Drill Stops from Ø4,8 implants to Ø6,0			7960

Instruments and surgical kit


Avient supplies high-precision instruments designed to match implants and suitable for use with internal, external and conical connections. Avient's two surgical boxes allow practitioners to choose the working system that best meets their needs.

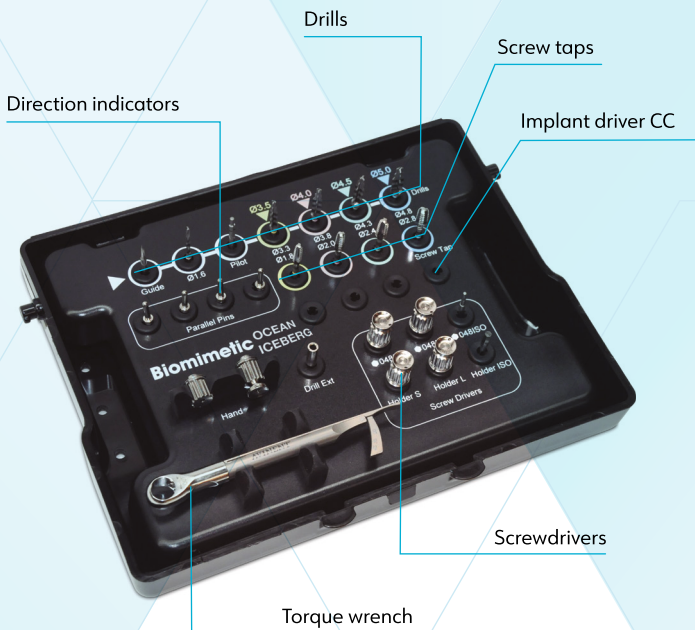

The sterilization cassette OCEAN/ICEBERG

stands out for its clear layout and attractive design, making it easy to use. The drilling sequence is clearly indicated by means of a simple colour code according to the diameter of the selected implant. All the pieces are placed in a sterilizable tray with a see-through lid, giving a clear view of the interior.

The MiniBox is versatile, as it allows practitioners to select a specific sequence and take everything required for the surgical procedure with them in a small container. The box is sterilizable and can hold all the items needed for inserting prostheses.

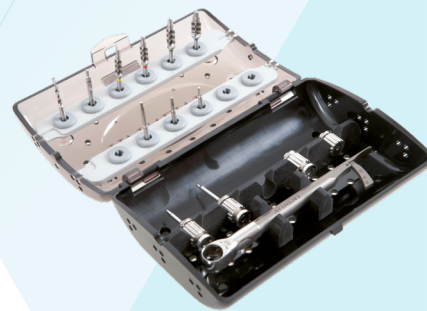

Advisable torque

TYPE	VALUE	
Mechanical	35 Ncm	Screw for single/Multiple abutment*
	30 Ncm	Screw for angled titanium base**
	30 Ncm	Screw for angulation correction G2 (max. 30°)**
	20 Ncm	Screw for angulation correction G1 (max. 20°)**
	15 Ncm	Screw transepithelial angled abutment
	15 Ncm	Prosthetic screw for transepithelial
	35 Ncm	Transepithelial abutment (Uniblock / 2 parts)
	30 Ncm	LOCATOR® / LOCATOR R-Tx® Abutment
	25 Ncm	RHEIN83® Abutment (OT Equator)
	15 Ncm	Temporary Abutment Ti
Manual	≈8-15 Ncm	Scan Abutment
		Impression coping open/closed tray engaging
		Healing Abutment Ti
		Healing cap

* Regarding: Titanium base, Cemented abutment and Cemented angled abutment, Castable CoCr Base. Included: Gold screw.

** Except Transep. 4.8 of M1.40 which is 15 Ncm.

Drilling speed biological protocol

	rpm
Guide drill	800 - 1.200
Drill ø 1,6 mm	800 - 1.200
Pilot drill	600 - 800
* Drill ø 2,0 - 3,3 mm	150 - 300
* Drill ø 2,2 - 3,8 mm	150 - 300
* Drill ø 2,8 - 4,3 mm	150 - 300
* Drill ø 3,2 - 4,8 mm	150 - 300
* Drill ø 2,4 - 3,3 mm	150 - 300
* Drill ø 3,0 - 3,7 mm	150 - 300
* Drill ø 3,8 - 4,3 mm	150 - 300
* Drill ø 4,1 - 4,7 mm	150 - 300
Screw Tap	20

* The biological drilling at low revolutions (between 50 and 100 rpm), allows to collect autologous bone as shown in the scientific literature.

Maximum recommended torque for implant insertion: 45-50 Ncm

Maximum recommended speed for implant insertion: 20 rpm

Drill-bit length and marking


Avinent drills carry laser markings to improve visibility during osteotomy and follow a colour code according to the diameter of the implant. The marking corresponds to the length of the implant in crestal placement, but the distances are not absolute from the tip of the instrument to the mark. The length of the drill tip is not included in the depth mark, so this distance must be taken into account when planning treatment and in carrying out the osteotomy.

Drilling speed standard protocol

	rpm
Guide drill	800 - 1.200
Drill ø 1,6 mm	800 - 1.200
Pilot drill	600 - 800
Drill ø 2,0 - 3,3 mm	200 - 400
Drill ø 2,2 - 3,8 mm	200 - 400
Drill ø 2,8 - 4,3 mm	200 - 400
Drill ø 3,2 - 4,8 mm	200 - 400
Drill ø 2,4 - 3,3 mm	200 - 400
Drill ø 3,0 - 3,7 mm	200 - 400
Drill ø 3,8 - 4,3 mm	200 - 400
Drill ø 4,1 - 4,7 mm	200 - 400
Screw Tap	20

Maximum recommended torque for implant insertion: 45-50 Ncm

Maximum recommended speed for implant insertion: 20 rpm

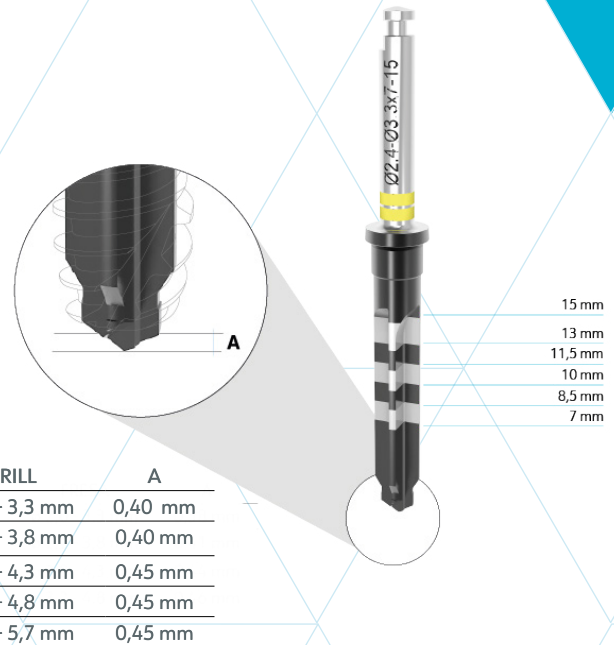


Accessories CC/CC.I

Implant handle



	REF.
L	2891
S	1878

Implant driver



	REF.
3,5 S	2981
3,5 L	2984
4,1 S	2982
4,1 L	2985

Platform indicators

To make life easier for our costumers, Avinent screws attachments follow the color code od the implant platform.



Platform
Ø 3,5 mm



Platform
Ø 4,1 mm

* For any additional information and instrument maintenance instructions, please check www.avinent.com

Avinent Biological drilling protocol

The Avinent surgical drilling protocol for the ICEBERG system is suitable for all bone types. The system includes drill bits with an external shape featuring three diameters and straight cut to match the design of the implant. The finish of the drills makes it easier to locate the marks that indicate length during surgery. The biological drilling at low revolutions (between 50 and 100 rpm), allows to collect autologous bone as shown in the scientific literature.

The implant is designed so that the BAS surface treated part must be placed juxtaosseously and the polished part of 1.8 mm, transmucosally according to the clinical criteria.

These drills incorporate an optimized cut that guarantees better precision and efficiency in surgical procedures. In addition, DLC Treatment (Diamond-Like Carbon) technology has been integrated, which results in a type of coating that reduces wear, minimizes friction and extends the useful life of the drills.

* Hard bone drills are identified with two color indicators.

Implant ø 3,5 mm

Ref.	Guide drill	Drill ø1,6 mm	Pilot drill ø1,6 - 2,4 mm	Drill ø 2,0 - 3,3 mm	Drill ø 2,4 - 3,3 mm	Screw tap	Implant
	0188	2046	2047	2048	3311 Option 1	2687 Option 2	
BONE TYPE III-IV							
BONE TYPE I-II							

Implant ø 4,0 mm

Ref.	Guide drill	Drill ø1,6 mm	Pilot drill ø1,6 - 2,4 mm	Drill ø 2,0 - 3,3 mm	Drill ø 2,2 - 3,8 mm	Drill ø 3,0 - 3,7 mm	Screw tap	Implant
	0188	2046	2047	2048	2049	3312 Option 1	2688 Option 2	
BONE TYPE III-IV								
BONE TYPE I-II								



Implant ø 4,5 mm

Ref.	0188	2046	2047	2048	2049	2050	3313	2689	
	BONE TYPE III-IV						Option 1	Option 2	
	BONE TYPE I-II								

Implant ø 5,0 mm

Ref.	0188	2046	2047	2048	2049	2050	2051	3314	2690	
	BONE TYPE III-IV						Option 1	Option 2		
	BONE TYPE I-II									

Avinent Standard drilling protocol

The Avinent ICEBERG system surgical drilling protocol is suitable for all bone types. The system offers conical drills that adapt to the design of the implant. The finish of the drills makes it easy to locate the length indicator marks during surgery. Biological milling at low revolutions (between 50 and 100 rpm) allows autologous bone to be harvested, as shown in the scientific literature.

The implant is designed so that the treated part with the BAS surface being placed juxtassosseous and the

polished 1.8 mm part transmucosally according to the clinical criteria.

These drills incorporate an optimized cut that guarantees better precision and efficiency in surgical procedures. In addition, DLC Treatment (Diamond-Like Carbon) technology has been integrated, which results in a type of coating that reduces wear, minimizes friction and extends the useful life of the drills.

* Hard bone drills are identified with two color indicators.

Implante ø 3,5 mm

Ref.	Guide drill	Drill ø1,6 mm	Pilot drill ø1,6 - 2,4 mm	Drill ø2,0 - 3,3 mm	Drill ø2,4 - 3,3 mm	Screw tap	Implant	
	0188	2046	2047	8032	8037	2687		
BONE TYPE III-IV							Option 1 Option 2	
BONE TYPE I-II								

Implante ø 4,0 mm

Ref.	Guide drill	Drill ø1,6 mm	Pilot drill ø1,6 - 2,4 mm	Drill ø2,0 - 3,3 mm	Drill ø2,2 - 3,8 mm	Drill ø3,0 - 3,7 mm	Screw tap	Implant
	0188	2046	2047	8032	8033	8038	2688	
BONE TYPE III-IV							Option 1 Option 2	
BONE TYPE I-II								



Implante ø 4,5 mm

Ref.	0188	2046	2047	8032	8033	8034	8039	2689	
	BONE TYPE III-IV						Option 1	Option 2	
	BONE TYPE I-II								

Implante ø 5,0 mm

Ref.	0188	2046	2047	8032	8033	8034	8035	8040	2690	
	BONE TYPE III-IV						Option 1	Option 2		
	BONE TYPE I-II									

Sterilization and packaging



Avinent implants are subjected to a sterilization process in accordance with the requirements of the CE mark for medical device. Avinent supplies its implants in packaging that is easily identified by a simple colour code. The vial cap comes in different colours according to the diameter of the implant and has a sticker indicating the type of connection and the diameter and length of the implant.

The Avinent implant system is sold in a sterile blister pack, which ensures that the implant is fully protected until the given expiry date, so long as it is stored in suitable conditions.


Avinent supplies labeling with all its products that ensure every item can be properly traced by means of stickers that can be used in the patient's clinical history or in any other documentation required.



Blister pack (front and back)



Vial



Opening the vial



Implant



Cover screw

Opening the packaging

- Open the box and take out the blister pack.
- Open the blister pack and leave the vial containing the implant in the sterile working area, avoiding contact with any item that is not sterile. The sterile blister pack must not be opened prior to use.
- Open the vial by gripping the coloured cap with one hand while holding the transparent part in the other.
- Fit the implant driver into the implant.
- Press to make a tight fit and raise the implant set slightly.
- The cover screw is inside the coloured cap.

Information on the box

Rx only



Biomimetic ICEBERG



Manufacturer:
AVINENT Implant System S.L.U.
Pol. Ind. Santa Anna I, 08251 Santpedor (Barcelona) Spain.



ifu.avinent.com



Implant box label

Implant CC.I
ø 3.5 x 10 (3.5) Ti
REF 5900

ES Implante
PT Implante
FR Implant

(01) 08435452001046

(10) XXXXX

(17) AAMMDD

LOT XXXX

USE BY AAAA-MM-DD



Labels that make the product traceable

AVINENT
Implant CC.I ø 3.5 x 10 (3.5)

REF 5900 LOT XXXX

GTIN 08435452001046

STERILE R AAAA-MM-DD



AVINENT
Implant CC.I ø 3.5 x 10 (3.5)

REF 5900 LOT XXXX

GTIN 08435452001046

STERILE R AAAA-MM-DD



AVINENT
Implant CC.I ø 3.5 x 10 (3.5)

REF 5900 LOT XXXX

GTIN 08435452001046

STERILE R AAAA-MM-DD




AVINENT
Purchasing / Compra

REF 5900

LOT XXXX

Implant CC.I	ICEBERG conical connection indicator
ø 3.5 x 10 (3.5)	Diameter x length (implant holder)
Ti	Titanium
REF 5900	Reference number
LOT xxxxxx	Batch code
AAAA-MM-DD	Expiry date
STERILE R	Sterile. Sterilization method: radiation
ifu.avinent.com	Consult instructions for use
	Manufacturer
CE	CE Mark NB num 0197. TÜV Rheinland
Rx only	(For the USA only) CAUTION: Federal law restricts this device to sale by or on the order of a physician
(01) 08435452001046 (10) XXXXX (17) AAMMDD	UDI (Unique Device Identifier Carrier)
	Do not re-use
	Do not resterilize

Avinent Guided surgery

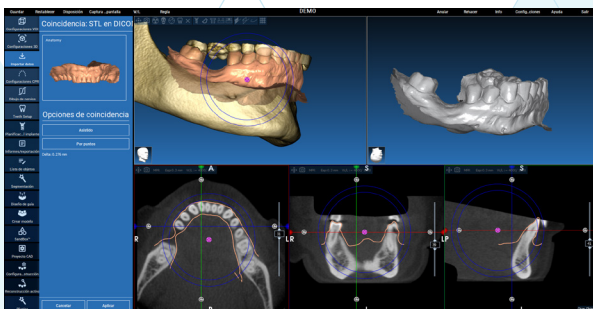

Avinent Guided Surgery


- Surgical Guide Box 3DIEMME®
- Implant planning software with Real Guide®

CT or CBCT Scanners. Available libraries for:

- NewTom
- Carestream
- (More coming soon)

Surgical motors

Avinent offers a wide range of surgical motors designed for many clinical applications, produced by leading brands in the industry. Intended to simplify daily practice and for multiple users, they can be adapted to suit each practitioner's needs by allowing the entire drilling sequence to be customised. Our surgical motors are ergonomically designed, easy to use and significantly help to reduce tiredness. They give implantology specialists a surgical unit for everyday use in safely carrying out oral procedures. All the surgical motors have been designed with the aim of minimising size and weight, to improve the balance of the instrument and motor in the practitioner's hand and thereby reduce tiredness during long treatments.

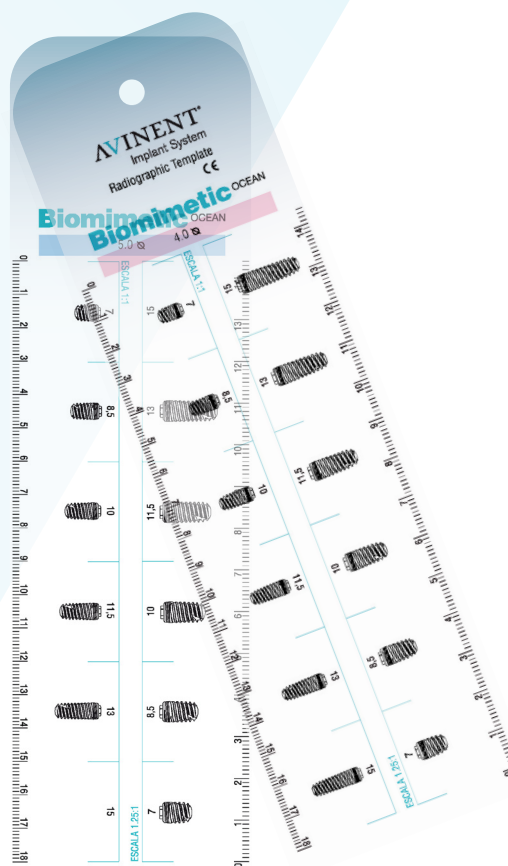

Radiographic template

The radiographic template is a guide to help practitioners precisely select the appropriate implant diameter and length.

To adapt it to the proportions of the x-ray, the dimensions of the implant are shown at a scale 1:1 and 1.25:1.

Bien Air[®]
Dental

NSK

Product index

REF.	DESCRIPTION		REF.	DESCRIPTION	
0188	Pointed drill	878	5602	Implant CC.I 3,5 x 13 (3,5)	4
0263	Screwdriver gold screw ISO 1797	6	5903	Implant CC.I 3,5 x 15 (3,5)	4
	Screwdriver Rhein 83 abutment		5904	Implant CC.I 4,0 x 7 (3,5)	4
0267	Screwdriver grooved screw ISO 1797	6	5905	Implant CC.I 4,0 x 8,5 (3,5)	4
0274	Screwdriver S (048)	7	5906	Implant CC.I 4,0 x 10 (3,5)	4
0275	Screwdriver L (048)	7	5907	Implant CC.I 4,0 x 11,5 (3,5)	4
0277	Screwdriver ISO 1797 L (048)	6	5908	Implant CC.I 4,0 x 13 (3,5)	4
0278	Implant driver S (2.5)	7	5909	Implant CC.I 4,0 x 15 (3,5)	4
0295	Torque wrench	6	5910	Implant CC.I 4,5 x 7 (4,1)	5
0299	Implant driver L (2.5)	7	5911	Implant CC.I 4,5 x 8,5 (4,1)	5
0328	Screwdriver transepithelial abutment ISO 1797 S	6	5912	Implant CC.I 4,5 x 10 (4,1)	5
0526	MiniBox	6	5913	Implant CC.I 4,5 x 11,5 (4,1)	5
0644	Screwdriver ISO 1797 S (048)	6	5914	Implant CC.I 4,5 x 13 (4,1)	5
0645	Screwdriver ISO 1797 XL (048)	6	5915	Implant CC.I 4,5 x 15 (4,1)	5
0648	Screwdriver transepithelial angled abutment ISO 1797 L (0,48)	6	5917	Implant CC.I 5,0 x 7 (4,1)	5
K1589B204	Drill extension	7	5918	Implant CC.I 5,0 x 8,5 (4,1)	5
0723	Screwdriver impression coping closed tray ISO 1797	6	5919	Implant CC.I 5,0 x 10 (4,1)	5
0726	Screwdriver transepithelial abutment ISO 1797 L	6	5920	Implant CC.I 5,0 x 11,5 (4,1)	5
0790	Handle ISO 1797 L	7	5922	Healing abutment CC.I 3,5 x 2	4
0791	Handle ISO 1797 S	7	5923	Healing abutment CC.I 3,5 x 3	4
0804	Screwdriver transepithelial angled abutment ISO 1797 S(0,48)	6	5924	Healing abutment CC.I 3,5 x 5	4
1763	Sterilization cassette OCEAN	6	5925	Healing abutment CC.I 4,1 x 4 x 2	5
1810	Direction indicator \varnothing 1,5 - \varnothing 2,3	7	5926	Healing abutment CC.I 4,1 x 4 x 3	5
1878	Implant handle S	7	5927	Healing abutment CC.I 4,1 x 4 x 5	5
2046	Twist drill \varnothing 1,6 x 7 - 15	7	5928	Anatomic healing abutment CC.I 3,5 x 4 x 2	4
2047	Pilot drill \varnothing 1,6 - \varnothing 2,4	7	5929	Anatomic healing abutment CC.I 3,5 x 4 x 3	4
2048	Drill \varnothing 2,0 - \varnothing 3,3 x 7 - 15	7	5930	Anatomic healing abutment CC.I 3,5 x 4 x 5	4
2049	Drill \varnothing 2,2 - \varnothing 3,8 x 7 - 15	7	5931	Anatomic healing abutment CC.I 3,5 x 5 x 2	4
2050	Drill \varnothing 2,8 - \varnothing 4,3 x 7 - 15	7	5932	Anatomic healing abutment CC.I 3,5 x 5 x 3	4
2051	Drill \varnothing 3,2 - \varnothing 4,8 x 7 - 13	7	5933	Anatomic healing abutment CC.I 3,5 x 5 x 5	4
2687	Screw tap 3,5 mm	7	5934	Anatomic healing abutment CC.I 4,1 x 5 x 2	5
2688	Screw tap 4,0 mm	7	5935	Anatomic healing abutment CC.I 4,1 x 5 x 3	5
2689	Screw tap 4,5 mm	7	5936	Anatomic healing abutment CC.I 4,1 x 5 x 5	5
2690	Screw tap 5,0 mm	7	5937	Anatomic healing abutment CC.I 4,1 x 6 x 2	5
2891	Implant handle L	7	5938	Anatomic healing abutment CC.I 4,1 x 6 x 3	5
2981	Implant driver ISO 1797 CC 3,5 S	6	5939	Anatomic healing abutment CC.I 4,1 x 6 x 5	5
2982	Implant driver ISO 1797 CC 4,1 S	6	6984	Drill Stop \varnothing 1.3-2.4L7	8
2984	Implant driver ISO 1797 CC 3,5 L	6	6985	Drill Stop \varnothing 1.3-2.4L8.5	8
2985	Implant driver ISO 1797 CC 4,1 L	6	6986	Drill Stop \varnothing 1.3-2.4L10	8
3311	Hard bone drill \varnothing 2,4 - \varnothing 3,3 x 7 - 15	7	6987	Drill Stop \varnothing 1.3-2.4L11.5	8
3312	Hard bone drill \varnothing 3,0 - \varnothing 3,7 x 7 - 15	7	6988	Drill Stop \varnothing 1.3-2.4L13	8
3313	Hard bone drill \varnothing 3,8 - \varnothing 4,3 x 7 - 15	7	6989	Drill Stop \varnothing 1.3-2.4L15	8
3314	Hard bone drill \varnothing 4,1 - \varnothing 4,7 x 7 - 13	7	6990	CORAL/OCEAN/ICEBERG Drill Stop \varnothing 2,8-3,3 L7	8
5184	Screwdriver for angulation correcting G2 24 mm	7	6991	CORAL/OCEAN/ICEBERG Drill Stop \varnothing 2,8-3,3 L8,5	8
5185	Screwdriver for angulation correcting G2 32 mm	7	6992	CORAL/OCEAN/ICEBERG Drill Stop \varnothing 2,8-3,3 L10	8
5900	Implant CC.I 3,5 x 10 (3,5)	4	6993	CORAL/OCEAN/ICEBERG Drill Stop \varnothing 2,8-3,3 L11,5	8
5901	Implant CC.I 3,5 x 11,5 (3,5)	4	6994	CORAL/OCEAN/ICEBERG Drill Stop \varnothing 2,8-3,3 L13	8
			6995	CORAL/OCEAN/ICEBERG Drill Stop \varnothing 2,8-3,3 L15	8
			6996	CORAL/OCEAN/ICEBERG Drill Stop \varnothing 3,2-3,8 L7	8

*The availability of the products in this catalog may vary depending on the country where you are based. Please contact your Avinent distributor for further information.

REF.	DESCRIPTION	
6997	CORAL/OCEAN/ICEBERG Drill Stop Ø3,2-3,8 L8,5	8
6998	CORAL/OCEAN/ICEBERG Drill Stop Ø3,2-3,8 L10	8
6999	CORAL/OCEAN/ICEBERG Drill Stop Ø3,2-3,8 L11,5	8
7000	CORAL/OCEAN/ICEBERG Drill Stop Ø3,2-3,8 L13	8
7001	CORAL/OCEAN/ICEBERG Drill Stop Ø3,2-3,8 L15	8
7002	CORAL/OCEAN/ICEBERG Drill Stop Ø3,6-4,3 L7	8
7003	CORAL/OCEAN/ICEBERG Drill Stop Ø3,6-4,3 L8,5	8
7004	CORAL/OCEAN/ICEBERG Drill Stop Ø3,6-4,3 L10	8
7005	CORAL/OCEAN/ICEBERG Drill Stop Ø3,6-4,3 L11,5	8
7006	CORAL/OCEAN/ICEBERG Drill Stop Ø3,6-4,3 L13	8
7007	CORAL/OCEAN/ICEBERG Drill Stop Ø3,6-4,3 L15	8
7008	CORAL/OCEAN/ICEBERG Drill Stop Ø4,2-4,8 L7	8
7009	CORAL/OCEAN/ICEBERG Drill Stop Ø4,2-4,8 L8,5	8
7010	CORAL/OCEAN/ICEBERG Drill Stop Ø4,2-4,8 L10	8
7011	CORAL/OCEAN/ICEBERG Drill Stop Ø4,2-4,8 L11,5	8
7012	CORAL/OCEAN/ICEBERG Drill Stop Ø4,2-4,8 L13	8
7013	OCEAN Drill Stop Ø5,7 L7	8
7014	OCEAN Drill Stop Ø5,7 L8,5	8
7015	OCEAN Drill Stop Ø5,7 L10	8
7016	OCEAN Drill Stop Ø5,7 L11,5	8
7959	Drill Stop Kit for implants up to Ø4.5	8
7960	Drill Stop Set for implants from Ø4.8 to Ø6.0	8
8032	Helical drill ø 2,0 - 3,3	14
8033	Helical drill ø 2,2 - 3,8	14
8034	Helical drill ø 2,8 - 4,3	14
8035	Helical drill ø 3,2 - 4,8	14
8037	Hard bone helical drill ø 2,0 - 3,3	14
8038	Hard bone helical drill ø 3,0 - 3,7	14
8039	Hard bone helical drill ø 3,8 - 4,3	14
8040	Hard bone helical drill ø 4,1 - 4,7	14



Carretera de Navarcles, 107
Pol. Industrial Santa Anna I
08251 Santpedor (Barcelona) - España
T. (+34) 93 827 34 65
www.avinent.com - avinent@avinent.com

AVINENT AUSTRALIA
australia@avinent.com

AVINENT BENELUX
benelux@avinent.com

AVINENT CANADA
canada@avinent.com

AVINENT COLOMBIA
colombia@avinent.com

AVINENT CROATIA
croatia@avinent.com

AVINENT FRANCE
france@avinent.com

AVINENT KUWAIT
kuwait@avinent.com

AVINENT LITHUANIA
lithuania@avinent.com

AVINENT POLAND
poland@avinent.com

AVINENT PORTUGAL
portugal@avinent.com

AVINENT ROMANIA
romania@avinent.com

AVINENT TAIWAN
taiwan@avinent.com

AVINENT UKRAINE
ukraine@avinent.com

AVINENT UNITED ARAB EMIRATES
uae@avinent.com

AVINENT UNITED KINGDOM
uk@avinent.com

AVINENT USA
usa@avinent.com

AVINENT VIETNAM
vietnam@avinent.com

AVINENT SAUDI ARABIA
ksa@avinent.com



Management
System
ISO 13485:2016
www.tuv.com

