


PRODUCT CATALOGUE

Biomimetic **OCEAN**

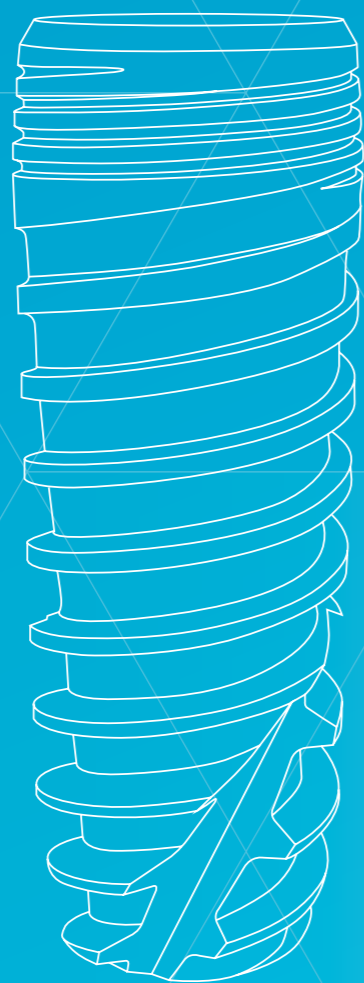


The OCEAN system is a new line that adds to the range of Avinent implants. This new system has all the innovative features of the CORAL implant, as well as new concepts to provide a solution to emerging clinical and prosthetic needs. The shape of the OCEAN system shows outstanding aesthetic results at tissue level.

CONTENTS

Surgical phase	4
EC External connection	4
IC Internal connection	6
IC Internal connection No Holder	8
CC Conical connection	10
Accessories	12
Drills stops	14
Instruments and surgical kit	15
Drilling speed	17
Drill-bit length and marking	17
Accessories CC and IC No Holder	17
Platform indicators	17
Avinent drilling biological protocol	18
Avinent drilling standard protocol	20
Sterilization and packaging	22
Avinent Guided Surgery	24
Micromotors	24
Radiographic template	24
Product index	25




Biomimetic OCEAN

EC




EXTERNAL CONNECTION

SURGICAL PHASE




	Platform Ø 3,5 mm				Platform Ø 4,1 mm			
	Ø 3,5 mm	Ref.	Ø 4,0 mm	Ref.	Ø 4,5 mm	Ref.	Ø 5,0 mm	Ref.
Implant 	-	-	4,0 x 7 mm	1562	4,5 x 7 mm	1568	5,0 x 7 mm	1574
	-	8144	4,0 x 8,5 mm	1563	4,5 x 8,5 mm	1569	5,0 x 8,5 mm	1575
	3,5 x 10 mm	1558	4,0 x 10 mm	1564	4,5 x 10 mm	1570	5,0 x 10 mm	1576
	3,5 x 11,5 mm	1559	4,0 x 11,5 mm	1565	4,5 x 11,5 mm	1571	5,0 x 11,5 mm	1577
	3,5 x 13 mm	1560	4,0 x 13 mm	1566	4,5 x 13 mm	1572	5,0 x 13 mm	1578
	3,5 x 15 mm	1561	4,0 x 15 mm	1567	4,5 x 15 mm	1573	-	-
Healing abutment 	4 x 3 mm	0030	4 x 3 mm	0030	4 x 3 mm	3363	4 x 3 mm	3363
	4 x 4 mm	0031	4 x 4 mm	0031	4 x 5 mm	3364	4 x 5 mm	3364
	4 x 5 mm	0032	4 x 5 mm	0032	4 x 7 mm	3365	4 x 7 mm	3365
	5 x 3 mm	0033	5 x 3 mm	0033	5 x 3 mm	0036	5 x 3 mm	0036
	5 x 4 mm	0034	5 x 4 mm	0034	5 x 4 mm	0037	5 x 4 mm	0037
	5 x 5 mm	0035	5 x 5 mm	0035	5 x 5 mm	0003	5 x 5 mm	0003
	-	-	-	-	5 x 7 mm	0038	5 x 7 mm	0038
Anatomic healing abutment 	5 x 3 mm	0171	5 x 3 mm	0171	5 x 3 mm	0174	5 x 3 mm	0174
	5 x 4 mm	0172	5 x 4 mm	0172	5 x 4 mm	0175	5 x 4 mm	0175
	5 x 5 mm	0173	5 x 5 mm	0173	5 x 5 mm	0176	5 x 5 mm	0176
	-	-	-	-	5 x 7 mm	0177	5 x 7 mm	0177

Biomimetic OCEAN



INTERNAL CONNECTION

SURGICAL PHASE

	Platform Ø 3,5 mm				Platform Ø 4,1 mm			
	Ø 3,5 mm	Ref.	Ø 4,0 mm	Ref.	Ø 4,5 mm	Ref.	Ø 5,0 mm	Ref.
Implant 	3,5 x 7 mm	8150	4,0 x 7 mm	1583	4,5 x 7 mm	1589	5,0 x 7 mm	1595
	3,5 x 8,5 mm	8149	4,0 x 8,5 mm	1584	4,5 x 8,5 mm	1590	5,0 x 8,5 mm	1596
	3,5 x 10 mm	1579	4,0 x 10 mm	1585	4,5 x 10 mm	1591	5,0 x 10 mm	1597
	3,5 x 11,5 mm	1580	4,0 x 11,5 mm	1586	4,5 x 11,5 mm	1592	5,0 x 11,5 mm	1598
	3,5 x 13 mm	1581	4,0 x 13 mm	1587	4,5 x 13 mm	1593	5,0 x 13 mm	1599
	3,5 x 15 mm	1582	4,0 x 15 mm	1588	4,5 x 15 mm	1594	-	-
Anatomic healing abutment 	3,5 x 3 mm	3370	3,5 x 3 mm	3370	3,5 x 3 mm	3370	3,5 x 3 mm	3370
	3,5 x 5 mm	3371	3,5 x 5 mm	3371	3,5 x 5 mm	3371	3,5 x 5 mm	3371
	3,5 x 7 mm	3372	3,5 x 7 mm	3372	3,5 x 7 mm	3372	3,5 x 7 mm	3372
	4,5 x 2 mm	0465	4,5 x 2 mm	0465	4,5 x 2 mm	0465	4,5 x 2 mm	0465
	4,5 x 3 mm	0466	4,5 x 3 mm	0466	4,5 x 3 mm	0466	4,5 x 3 mm	0466
	4,5 x 4 mm	0467	4,5 x 4 mm	0467	4,5 x 4 mm	0467	4,5 x 4 mm	0467
	4,5 x 5 mm	0468	4,5 x 5 mm	0468	4,5 x 5 mm	0468	4,5 x 5 mm	0468
	4,5 x 7 mm	0469	4,5 x 7 mm	0469	4,5 x 7 mm	0469	4,5 x 7 mm	0469
	5,5 x 3 mm	0471	5,5 x 3 mm	0471	5,5 x 3 mm	0471	5,5 x 3 mm	0471
	5,5 x 4 mm	0472	5,5 x 4 mm	0472	5,5 x 4 mm	0472	5,5 x 4 mm	0472
	5,5 x 5 mm	0473	5,5 x 5 mm	0473	5,5 x 5 mm	0473	5,5 x 5 mm	0473
	5,5 x 7 mm	0474	5,5 x 7 mm	0474	5,5 x 7 mm	0474	5,5 x 7 mm	0474
	6,5 x 3 mm	2737	6,5 x 3 mm	2737	6,5 x 3 mm	2737	6,5 x 3 mm	2737
	6,5 x 4 mm	2727	6,5 x 4 mm	2727	6,5 x 4 mm	2727	6,5 x 4 mm	2727
	6,5 x 5 mm	2726	6,5 x 5 mm	2726	6,5 x 5 mm	2726	6,5 x 5 mm	2726
Aesthetic healing abutment 	4,5 x 2 mm	0607	4,5 x 2 mm	0607	4,5 x 2 mm	0607	4,5 x 2 mm	0607
	4,5 x 3 mm	0608	4,5 x 3 mm	0608	4,5 x 3 mm	0608	4,5 x 3 mm	0608
	4,5 x 4 mm	0609	4,5 x 4 mm	0609	4,5 x 4 mm	0609	4,5 x 4 mm	0609
	4,5 x 5 mm	0610	4,5 x 5 mm	0610	4,5 x 5 mm	0610	4,5 x 5 mm	0610
	4,5 x 6 mm	0611	4,5 x 6 mm	0611	4,5 x 6 mm	0611	4,5 x 6 mm	0611
	4,5 x 7 mm	0612	4,5 x 7 mm	0612	4,5 x 7 mm	0612	4,5 x 7 mm	0612

Biomimetic OCEAN






NO HOLDER



INTERNAL CONNECTION

SURGICAL PHASE

	Platform Ø 3,5 mm				Platform Ø 4,1 mm			
	Ø 3,5 mm	Ref.	Ø 4,0 mm	Ref.	Ø 4,5 mm	Ref.	Ø 5,0 mm	Ref.
Implant 	3,5 x 7 mm	8147	4,0 x 7 mm	8064	4,5 x 7 mm	8070	5,0 x 7 mm	8076
	3,5 x 8,5 mm	8148	4,0 x 8,5 mm	8065	4,5 x 8,5 mm	8071	5,0 x 8,5 mm	8077
	3,5 x 10 mm	8060	4,0 x 10 mm	8066	4,5 x 10 mm	8072	5,0 x 10 mm	8078
	3,5 x 11,5 mm	8061	4,0 x 11,5 mm	8067	4,5 x 11,5 mm	8073	5,0 x 11,5 mm	8079
	3,5 x 13 mm	8062	4,0 x 13 mm	8068	4,5 x 13 mm	8074	5,0 x 13 mm	8080
	3,5 x 15 mm	8063	4,0 x 15 mm	8069	4,5 x 15 mm	8075	-	-
Anatomic healing abutment 	3,5 x 3 mm	3370	3,5 x 3 mm	3370	3,5 x 3 mm	3370	3,5 x 3 mm	3370
	3,5 x 5 mm	3371	3,5 x 5 mm	3371	3,5 x 5 mm	3371	3,5 x 5 mm	3371
	3,5 x 7 mm	3372	3,5 x 7 mm	3372	3,5 x 7 mm	3372	3,5 x 7 mm	3372
	4,5 x 2 mm	0465	4,5 x 2 mm	0465	4,5 x 2 mm	0465	4,5 x 2 mm	0465
	4,5 x 3 mm	0466	4,5 x 3 mm	0466	4,5 x 3 mm	0466	4,5 x 3 mm	0466
	4,5 x 4 mm	0467	4,5 x 4 mm	0467	4,5 x 4 mm	0467	4,5 x 4 mm	0467
	4,5 x 5 mm	0468	4,5 x 5 mm	0468	4,5 x 5 mm	0468	4,5 x 5 mm	0468
	4,5 x 7 mm	0469	4,5 x 7 mm	0469	4,5 x 7 mm	0469	4,5 x 7 mm	0469
	5,5 x 3 mm	0471	5,5 x 3 mm	0471	5,5 x 3 mm	0471	5,5 x 3 mm	0471
	5,5 x 4 mm	0472	5,5 x 4 mm	0472	5,5 x 4 mm	0472	5,5 x 4 mm	0472
	5,5 x 5 mm	0473	5,5 x 5 mm	0473	5,5 x 5 mm	0473	5,5 x 5 mm	0473
	5,5 x 7 mm	0474	5,5 x 7 mm	0474	5,5 x 7 mm	0474	5,5 x 7 mm	0474
	6,5 x 3 mm	2737	6,5 x 3 mm	2737	6,5 x 3 mm	2737	6,5 x 3 mm	2737
	6,5 x 4 mm	2727	6,5 x 4 mm	2727	6,5 x 4 mm	2727	6,5 x 4 mm	2727
	6,5 x 5 mm	2726	6,5 x 5 mm	2726	6,5 x 5 mm	2726	6,5 x 5 mm	2726
Aesthetic healing abutment 	4,5 x 2 mm	0607	4,5 x 2 mm	0607	4,5 x 2 mm	0607	4,5 x 2 mm	0607
	4,5 x 3 mm	0608	4,5 x 3 mm	0608	4,5 x 3 mm	0608	4,5 x 3 mm	0608
	4,5 x 4 mm	0609	4,5 x 4 mm	0609	4,5 x 4 mm	0609	4,5 x 4 mm	0609
	4,5 x 5 mm	0610	4,5 x 5 mm	0610	4,5 x 5 mm	0610	4,5 x 5 mm	0610
	4,5 x 6 mm	0611	4,5 x 6 mm	0611	4,5 x 6 mm	0611	4,5 x 6 mm	0611
	4,5 x 7 mm	0612	4,5 x 7 mm	0612	4,5 x 7 mm	0612	4,5 x 7 mm	0612

Biomimetic OCEAN






NO HOLDER



CONICAL CONNECTION

SURGICAL PHASE

	Platform Ø 3,5 mm								Platform Ø 4,1 mm					
	Ø 3,5 mm	Ref.	Ø 4,0 mm	Ref.	Ø 4,5 mm	Ref.	Ø 5,0 mm	Ref.	Ø 4,5 mm	Ref.	Ø 5,0 mm	Ref.	Ø 6,0 mm	Ref.
Implant 	3,5 x 7 mm	8143	4,0 x 7 mm	2939	4,5 x 7 mm	6344	5,0 x 7 mm	6350	4,5 x 7 mm	2945	5,0 x 7 mm	2951	6,0 x 7 mm	3812
	3,5 x 8,5 mm	8144	4,0 x 8,5 mm	2940	4,5 x 8,5 mm	6345	5,0 x 8,5 mm	6351	4,5 x 8,5 mm	2946	5,0 x 8,5 mm	2952	6,0 x 8,5 mm	3938
	3,5 x 10 mm	2935	4,0 x 10 mm	2941	4,5 x 10 mm	6346	5,0 x 10 mm	6352	4,5 x 10 mm	2947	5,0 x 10 mm	2953	6,0 x 10 mm	3939
	3,5 x 11,5 mm	2936	4,0 x 11,5 mm	2942	4,5 x 11,5 mm	6347	5,0 x 11,5 mm	6353	4,5 x 11,5 mm	2948	5,0 x 11,5 mm	2954	6,0 x 11,5 mm	3814
	3,5 x 13 mm	2937	4,0 x 13 mm	2943	4,5 x 13 mm	6348	5,0 x 13 mm	6354	4,5 x 13 mm	2949	5,0 x 13 mm	2955	-	-
	3,5 x 15 mm	2938	4,0 x 15 mm	2944	4,5 x 15 mm	6349	-	-	4,5 x 15 mm	2950	-	-	-	-
Anatomic healing abutment (Single) 	4 x 3 mm	2988	4 x 3 mm	2988	4 x 3 mm	2988	4 x 3 mm	2988	5 x 3 mm	2998	5 x 3 mm	2998	5 x 3 mm	2998
	4 x 5 mm	2989	4 x 5 mm	2989	4 x 5 mm	2989	4 x 5 mm	2989	5 x 5 mm	2999	5 x 5 mm	2999	5 x 5 mm	2999
	-	-	-	-	4 x 7 mm	-	-	-	5 x 7 mm	3000	5 x 7 mm	3000	5 x 7 mm	3000
	5 x 3 mm	2990	5 x 3 mm	2990	5 x 3 mm	2990	5 x 3 mm	2990	6 x 3 mm	3470	6 x 3 mm	3470	6 x 3 mm	3470
	5 x 5 mm	2991	5 x 5 mm	2991	5 x 5 mm	2991	5 x 5 mm	2991	6 x 5 mm	3471	6 x 5 mm	3471	6 x 5 mm	3471
	5 X 7 mm	2992	5 X 7 mm	2992	5 x 7 mm	2992	5 X 7 mm	2992	6 x 7 mm	3472	6 x 7 mm	3472	6 x 7 mm	3472
Anatomic healing abutment (Multiple) 	4 x 3 mm	2993	4 x 3 mm	2993	4 x 3 mm	2993	4 x 3 mm	2993	5 x 3 mm	3473	5 x 3 mm	3473	5 x 3 mm	3473
	4 x 5 mm	2994	4 x 5 mm	2994	4 x 5 mm	2994	4 x 5 mm	2994	5 x 5 mm	3474	5 x 5 mm	3474	5 x 5 mm	3474
	-	-	-	-	-	-	-	-	5 x 7 mm	3008	5 x 7 mm	3008	5 x 7 mm	3008
	5 x 3 mm	2995	5 x 3 mm	2995	5 x 3 mm	2995	5 x 3 mm	2995	6 x 3 mm	3010	6 x 3 mm	3010	6 x 3 mm	3010
	5 x 5 mm	2996	5 x 5 mm	2996	5 x 5 mm	2996	5 x 5 mm	2996	6 x 5 mm	3011	6 x 5 mm	3011	6 x 5 mm	3011
	5 X 7 mm	2997	5 X 7 mm	2997	5 X 7 mm	2997	5 X 7 mm	2997	6 x 7 mm	3012	6 x 7 mm	3012	6 x 7 mm	3012











ACCESSORIES

	Ref.
Sterilization cassette OCEAN	1763
MiniBox	0526
Torque wrench	0295
Holding tool EC/IC	0651



Screwdrivers			
	Screwdriver L18 (Hex 1.20)	0644	
	Screwdriver L22 (Hex 1.20)	0277	
	Screwdriver L30 (Hex 1.20)	0645	
	Holder Driver EC/IC L18	2693	
	Holder Driver EC/IC L22	0300	
	Holder Driver WH EC/IC L22	2692	
	Screwdriver for Gold Screw/RHEIN83®	0263	
	Screwdriver for Grooved Screw	0267	
	Screwdriver Impr. Coping Closed Tray L20.5	0723	
	Screwdriver for Transep. Abutment L22	0328	
	Screwdriver for Transep. Abutment L30	0726	
	Screwdriver for Angled Transep. Abut. L25	0804	
	Screwdriver for Angled Transep. Abut. L30	0648	
	Implant Driver CC 3.5 & CC.I 3.5 (Short)	2981	
	Implant Driver CC 3.5 & CC.I 3.5 (Long)	2984	
	Implant Driver CC 4.1 & CC.I 4.1 (Short)	2982	
	Implant Driver CC 4.1 & CC.I 4.1 (Long)	2985	
	Implant Driver IC 3.5/4.1 (Short)	8082	
	Implant Driver IC 3.5/4.1 (Long)	8083	


Screwdriver handle		Handle ISO 1797 S		0791
		Handle ISO 1797 L		0790
Implant handle		Implant handle S		1878
		Implant handle L		2891
Monoblock screwdrivers		Screwdriver S (048)		0274
		Screwdriver L (048)		0275
Drills		Implant driver S (2.5)		0278
		Implant driver L (2.5)		0299
Drills		Pointed drill		0188
		Twist drill	1,6 x 7 - 15 mm	2046
		Pilot drill	1,6 - 2,4 mm	2047
		Drill	2,0 - 3,3 x 7 - 15 mm	2048
			2,2 - 3,8 x 7 - 15 mm	2049
			2,8 - 4,3 x 7 - 15 mm	2050
			3,2 - 4,8 x 7 - 13 mm	2051
			4,2 - 5,7 x 7 - 11,5 mm	3966
		Hard bone drill	2,4 - 3,3 x 7 - 15 mm	3311
			3,0 - 3,7 x 7 - 15 mm	3312
3,8 - 4,3 x 7 - 15 mm	3313			
4,1 - 4,7 x 7 - 13 mm	3314			
5,1 - 5,7 x 7 - 11,5 mm	3960			
Twist drill	2,0 - 3,3 x 7 - 15 mm	8032		
	2,2 - 3,8 x 7 - 15 mm	8033		
	2,8 - 4,3 x 7 - 15 mm	8034		
	3,2 - 4,8 x 7 - 13 mm	8035		
	4,2 - 5,7 x 7 - 11,5 mm	8036		
Hard bone twist drill	2,4 - 3,3 x 7 - 15 mm	8037		
	3,0 - 3,7 x 7 - 15 mm	8038		
	3,8 - 4,3 x 7 - 15 mm	8039		
	4,1 - 4,7 x 7 - 13 mm	8040		
	5,1 - 5,7 x 7 - 11,5 mm	8041		
Screw tap		Screw tap	3,5 mm	2687
			4,0 mm	2688
			4,5 mm	2689
			5,0 mm	2690
			6,0 mm	3963

Direction indicator		1,5 - 2,3 mm	1810
Drill extension ISO 1797			KI589B204
Drill stops		Ø1,3-2,4 L7 Ø1,3-2,4 L8,5 Ø1,3-2,4 L10 Ø1,3-2,4 L11,5 Ø1,3-2,4 L13 Ø1,3-2,4 L15	6984 6985 6986 6987 6988 6989
		Ø2,8-3,3 L7 Ø2,8-3,3 L8,5 Ø2,8-3,3 L10 Ø2,8-3,3 L11,5 Ø2,8-3,3 L13 Ø2,8-3,3 L15	6990 6991 6992 6993 6994 6995
		Ø3,2-3,8 L7 Ø3,2-3,8 L8,5 Ø3,2-3,8 L10 Ø3,2-3,8 L11,5 Ø3,2-3,8 L13 Ø3,2-3,8 L15	6996 6997 6998 6999 7000 7001
		Ø3,6-4,3 L7 Ø3,6-4,3 L8,5 Ø3,6-4,3 L10 Ø3,6-4,3 L11,5 Ø3,6-4,3 L13 Ø3,6-4,3 L15	7002 7003 7004 7005 7006 7007
		Ø4,2-4,8 L7 Ø4,2-4,8 L8,5 Ø4,2-4,8 L10 Ø4,2-4,8 L11,5 Ø4,2-4,8 L13	7008 7009 7010 7011 7012
		Ø5,7 L7 Ø5,7 L8,5 Ø5,7 L10 Ø5,7 L11,5	7013 7014 7015 7016
Drill Stops Kit for implants up to Ø4,5			7959
Drill Stops from Ø4,8 implants to Ø6,0			7960

Instruments and surgical kit


Avinent supplies high-precision instruments designed to match implants and suitable for use with internal, external and conical connections.

Avinent's two surgical boxes allow practitioners to choose the working system that best meets their needs.

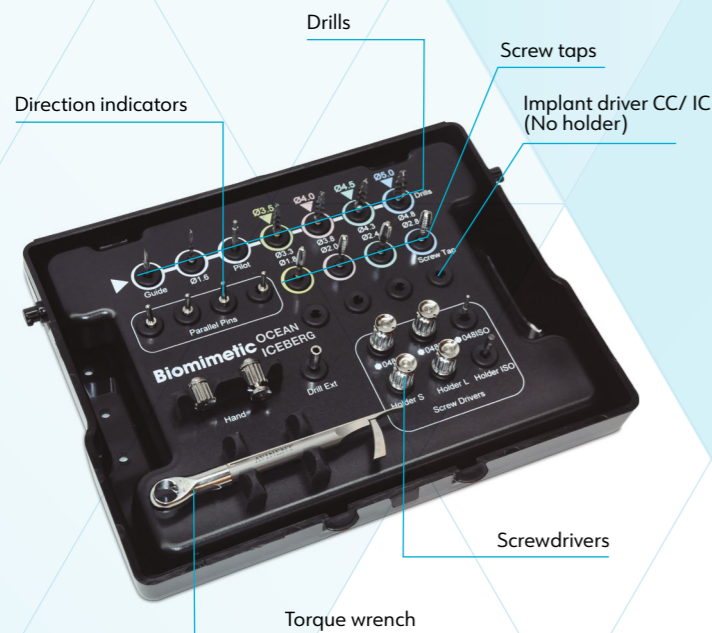

The sterilization cassette OCEAN stands out for its clear layout and attractive design, making it easy to use. The drilling sequence is clearly indicated by means of a simple colour code according to the diameter of the selected implant. All the pieces are placed in a sterilizable tray with a seethrough lid, giving a clear view of the interior.

The MiniBox is versatile, as it allows practitioners to select a specific sequence and take everything required for the surgical procedure with them in a small container. The box is sterilizable and can hold all the items needed for inserting prostheses.

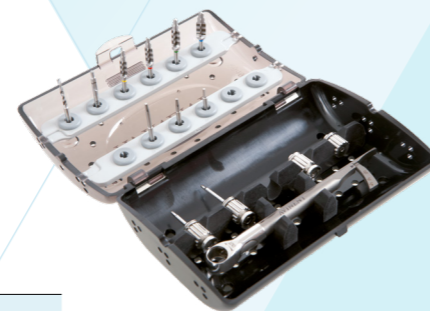

Advisable torque

TYPE	VALUE	
Mechanical	35 Ncm	Screw for single/Multiple abutment*
	30 Ncm	Screw for angled titanium base**
	30 Ncm	Screw for angulation correction G2 (max. 30°)**
	20 Ncm	Screw for angulation correction G1 (max. 20°)**
	15 Ncm	Screw transepithelial angled abutment
	15 Ncm	Prosthetic screw for transepithelial
	35 Ncm	Transepithelial abutment (Uniblock / 2 parts)
	30 Ncm	LOCATOR® / LOCATOR R-Tx® Abutment
25 Ncm	RHEIN83® Abutment (OT Equator)	
15 Ncm	Temporary Abutment Ti	
Manual	≈8-15 Ncm	Scan Abutment
		Impression coping open/closed tray engaging
		Healing Abutment Ti
		Healing cap

* Regarding: Titanium base, Cemented abutment and Cemented angled abutment, Castable CoCr Base. Included: Gold screw.

** Except Transep. 4.8 of M1.40 which is 15 Ncm.

Drilling speed biological protocol

	rpm
Guide drill	800 - 1.200
Drill ø 1,6 mm	800 - 1.200
Pilot drill	600 - 800
* Drill ø 2,0 - 3,3 mm	150 - 300
* Drill ø 2,2 - 3,8 mm	150 - 300
* Drill ø 2,8 - 4,3 mm	150 - 300
* Drill ø 3,2 - 4,8 mm	150 - 300
* Drill ø 2,4 - 3,3 mm	150 - 300
* Drill ø 3,0 - 3,7 mm	150 - 300
* Drill ø 3,8 - 4,3 mm	150 - 300
* Drill ø 4,1 - 4,7 mm	150 - 300
* Drill ø 4,2 - 5,7 mm	150 - 300
* Drill ø 5,1 - 5,7 mm	150 - 300
Screw Tap	20

* The biological drilling at low revolutions (between 50 and 100rpm), allows to collect autologous bone as shown in the scientific literature.

Maximum recommended torque for implant insertion: 45-50 Ncm

Maximum recommended speed for implant insertion: 20 rpm

Drill-bit length and marking


Avinent drills carry laser markings to improve visibility during osteotomy and follow a colour code according to the diameter of the implant. The marking corresponds to the length of the implant in crestal placement, but the distances are not absolute from the tip of the instrument to the mark. The length of the drill tip is not included in the depth mark, so this distance must be taken into account when planning treatment and in carrying out the osteotomy.

Drilling speed standard protocol

	rpm
Guide drill	800 - 1.200
Drill ø 1,6 mm	800 - 1.200
Pilot drill	600 - 800
Drill ø 2,0 - 3,3 mm	200 - 400
Drill ø 2,2 - 3,8 mm	200 - 400
Drill ø 2,8 - 4,3 mm	200 - 400
Drill ø 3,2 - 4,8 mm	200 - 400
Drill ø 2,4 - 3,3 mm	200 - 400
Drill ø 3,0 - 3,7 mm	200 - 400
Drill ø 3,8 - 4,3 mm	200 - 400
Drill ø 4,1 - 4,7 mm	200 - 400
Drill ø 4,2 - 5,7 mm	200 - 400
Drill ø 5,1 - 5,7 mm	200 - 400
Screw Tap	20

Maximum recommended torque for implant insertion: 45-50 Ncm

Maximum recommended speed for implant insertion: 20 rpm

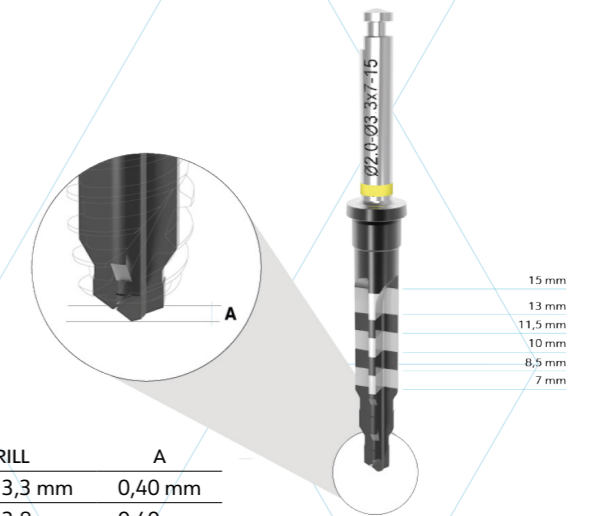


DRILL	A
ø 2,0 - 3,3 mm	0,40 mm
ø 2,2 - 3,8 mm	0,40 mm
ø 2,8 - 4,3 mm	0,45 mm
ø 3,2 - 4,8 mm	0,45 mm
ø 4,2 - 5,7 mm	0,45 mm

Accessories CC and IC No Holder

Implant handle	REF.
L	2891
S	1878
Implant driver for CC	REF.
3,5 S	2981
3,5 L	2984
4,1 S	2982
4,1 L	2985
Implant driver for IC (No Holder)	
3,5/4,1 S	8082
3,5/4,1 L	8083

Platform indicators

To make life easier for our costumers, Avinent screws attachments follow the color code of the implant platform (Only applicable to CC connection)

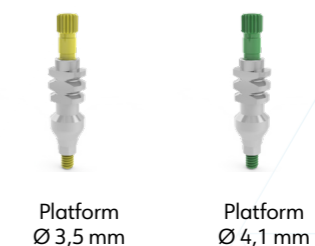

Platform
Ø 3,5 mm

Platform
Ø 4,1 mm

* For any additional information and instrument maintenance instructions, please check www.avinent.com

Avent Biological drilling protocol


The Avent surgical drilling protocol for the OCEAN system is suitable for all bone types. The system offers conical drills that adapt to the design of the implant. The finish of the drills makes it easier to locate the marks that indicate length during surgery. The biological drilling at low revolutions (between 50 and 100rpm), allows to collect autologous bone as shown in the scientific literature. Due to the surface treatment of the Avent implant up to the platform level, it is advisable to leave the implant

at the juxtaosseous or subcrestal level according to clinical criteria.


These drills incorporate an optimized cut that guarantees better precision and efficiency in surgical procedures. In addition, DLC Treatment (Diamond-Like Carbon) technology has been integrated, which results in a type of coating that reduces wear, minimizes friction and extends the lifetime of the drills.

* Hard bone drills are identified with two color indicators.


Implant ø 3,5 mm

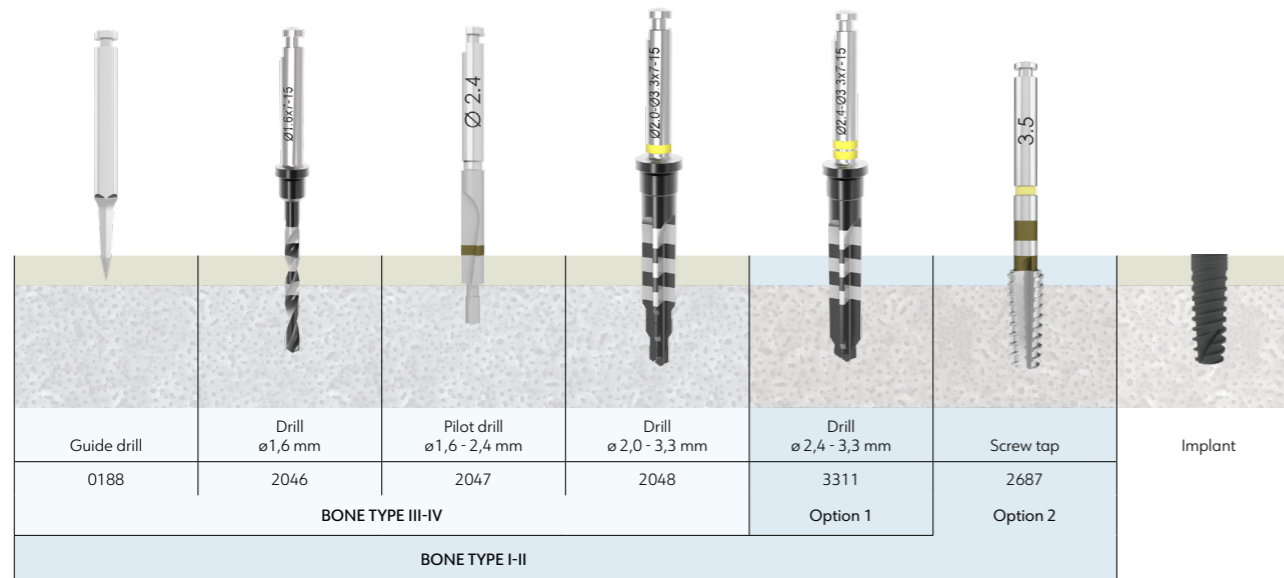


Implant ø 4,0 mm

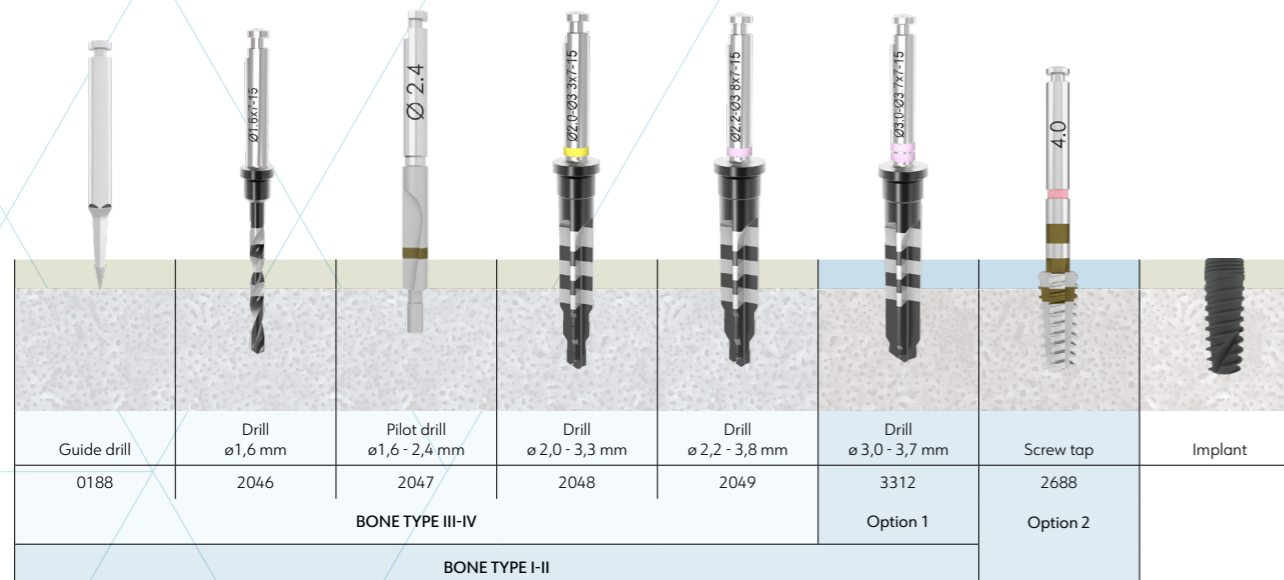


Implant ø 4,5 mm

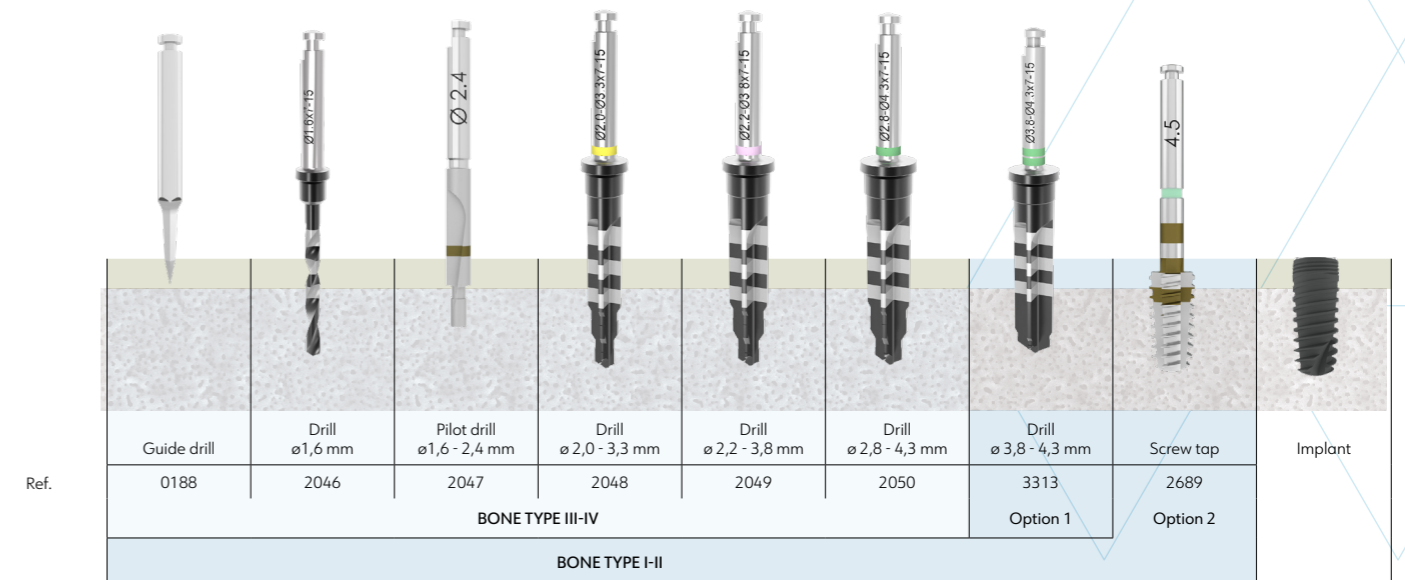

Implant ø 5,0 mm

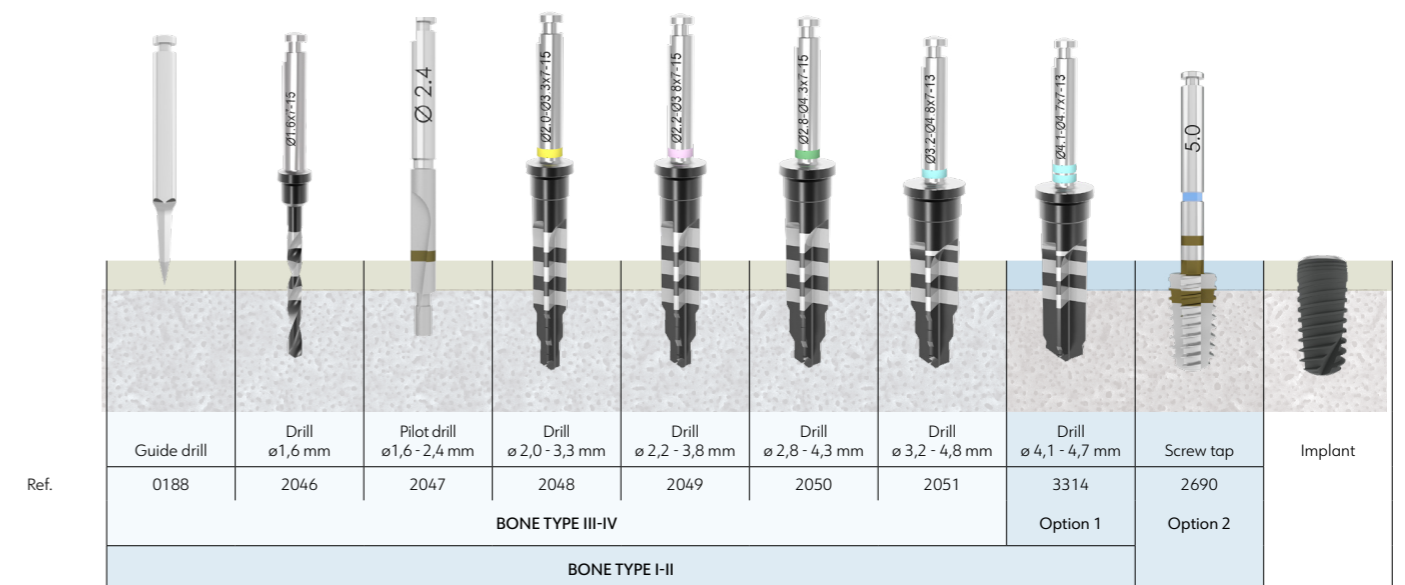

Implant ø 6,0 mm

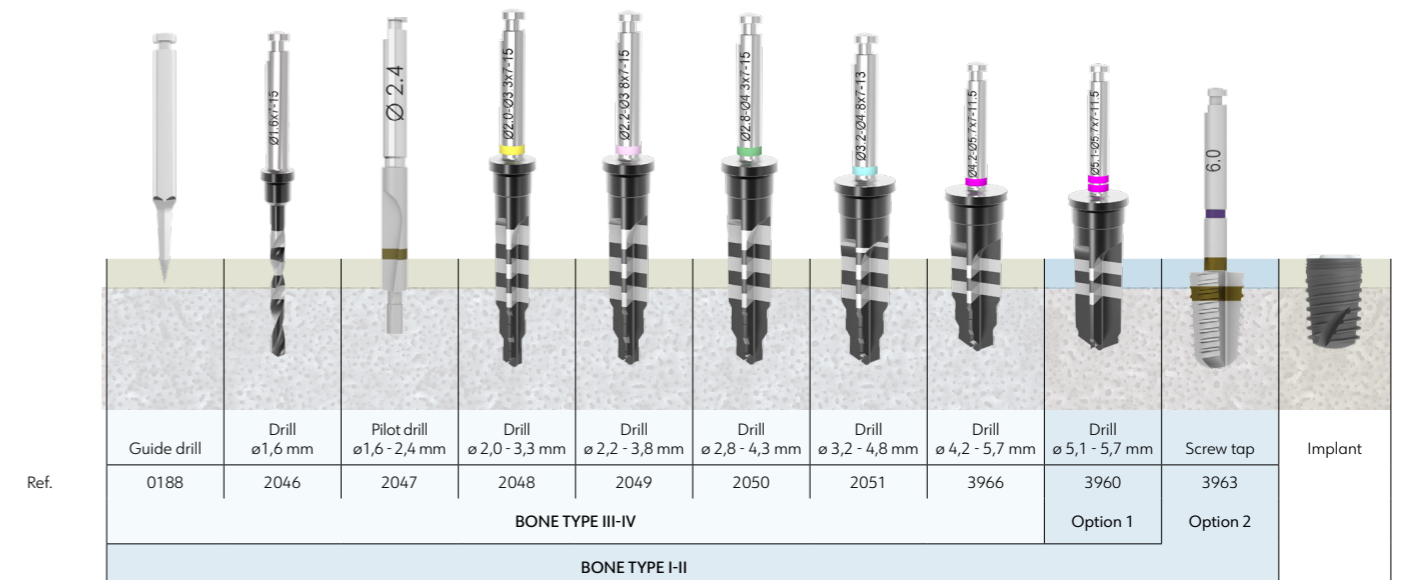

Aivent Standard drilling protocol

The Aivent drilling protocol for inserting OCEAN system implants is based on the anatomical and morphological characteristics of the bone to be worked on, the aim being to achieve satisfactory primary stability and a good bone-implant contact percentage, key factors for good osseointegration. The diameter of the helicoidal drills in the system is related to the core of the implant to be inserted. Hence it is advisable to use the system's drilling sequence and instruments.

The finish of the drills makes it easier to locate the marks that indicate length during surgery. Due to the fact that the surface treatment of the Aivent implant extends to the level of the platform, it is advisable to leave the Implant at juxtaosseous or subcrestal level according to clinical criteria.

These drills incorporate an optimized cut that guarantees better precision and efficiency in surgical procedures. In addition, DLC Treatment (Diamond-Like Carbon) technology has been integrated, which results in a type of coating that reduces wear, minimizes friction and extends the lifetime of the drills.

* Hard bone drills are identified with two color indicators.

Implant ø 3,5 mm

	Guide drill	Drill ø1,6 mm	Pilot drill ø1,6 - 2,4 mm	Drill ø 2,0 - 3,3 mm	Drill ø 2,4 - 3,3 mm	Screw tap	Implant
Ref.	0188	2046	2047	8032	8037	2687	
	BONE TYPE III-IV				Option 1	Option 2	
	BONE TYPE I-II						

Implant ø 4,0 mm

	Guide drill	Drill ø1,6 mm	Pilot drill ø1,6 - 2,4 mm	Drill ø 2,0 - 3,3 mm	Drill ø 2,2 - 3,8 mm	Drill ø 3,0 - 3,7 mm	Screw tap	Implant
Ref.	0188	2046	2047	8032	8033	8038	2688	
	BONE TYPE III-IV				Option 1	Option 2		
	BONE TYPE I-II							

Implant ø 4,5 mm

	Guide drill	Drill ø1,6 mm	Pilot drill ø1,6 - 2,4 mm	Drill ø 2,0 - 3,3 mm	Drill ø 2,2 - 3,8 mm	Drill ø 2,8 - 4,3 mm	Drill ø 3,8 - 4,3 mm	Screw tap	Implant
Ref.	0188	2046	2047	8032	8033	8034	8039	2689	
	BONE TYPE III-IV						Option 1	Option 2	
	BONE TYPE I-II								

Implant ø 5,0 mm

	Guide drill	Drill ø1,6 mm	Pilot drill ø1,6 - 2,4 mm	Drill ø 2,0 - 3,3 mm	Drill ø 2,2 - 3,8 mm	Drill ø 2,8 - 4,3 mm	Drill ø 3,2 - 4,8 mm	Drill ø 4,1 - 4,7 mm	Screw tap	Implant
Ref.	0188	2046	2047	8032	8033	8034	8035	8040	2690	
	BONE TYPE III-IV							Option 1	Option 2	
	BONE TYPE I-II									

Implant ø 6,0 mm

	Guide drill	Drill ø1,6 mm	Pilot drill ø1,6 - 2,4 mm	Drill ø 2,0 - 3,3 mm	Drill ø 2,2 - 3,8 mm	Drill ø 2,8 - 4,3 mm	Drill ø 3,2 - 4,8 mm	Drill ø 4,2 - 5,7 mm	Drill ø 5,1 - 5,7 mm	Screw tap	Implant
Ref.	0188	2046	2047	8032	8033	8034	8035	8036	8041	3963	
	BONE TYPE III-IV								Option 1	Option 2	
	BONE TYPE I-II										


Sterilization and packaging



Avinent implants are subjected to a sterilization process in accordance with the requirements of the CE mark for medical device. Avinent supplies its implants in packaging that is easily identified by a simple colour code. The vial cap comes in different colours according to the diameter of the implant and has a sticker indicating the type of connection and the diameter and length of the implant.

The Avinent implant system is sold in a sterile blister pack, which ensures that the implant is fully protected until the given expiry date, so long as it is stored in suitable conditions.

Avinent supplies labeling with all its products that ensure every item can be properly traced by means of stickers that can be used in the patient's clinical history or in any other documentation required.

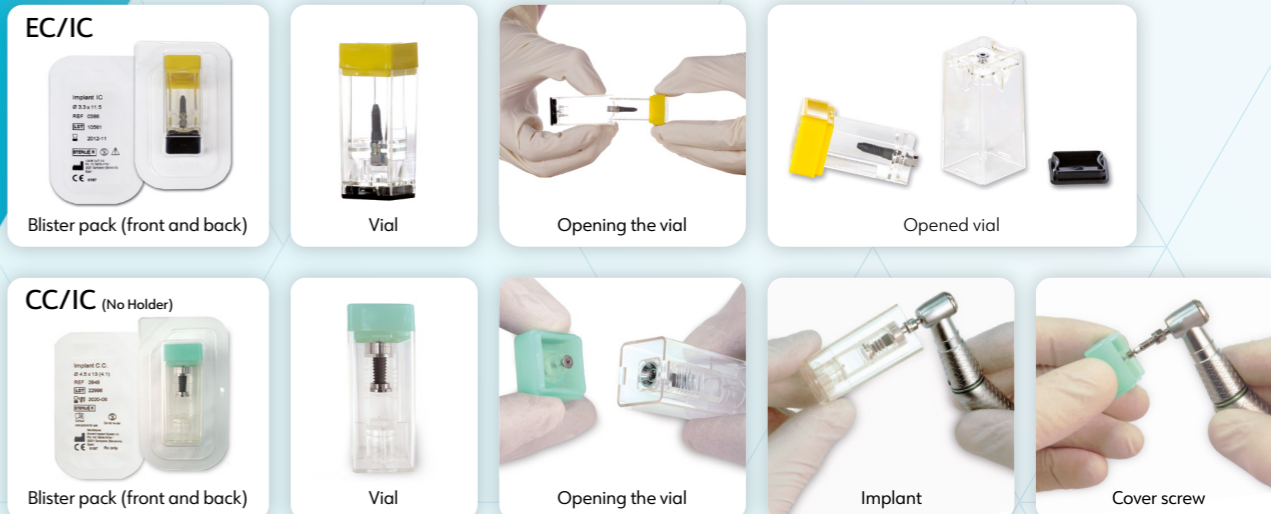


Opening the packaging

- Open the box and take out the blister pack.
- Open the blister pack and leave the vial containing the implant in the sterile working area, avoiding contact with any item that is not sterile. The sterile blister pack must not be opened prior to use.
- Open the vial by gripping the coloured cap with one hand while holding the transparent part in the other.
- EC/IC: Fit the implant driver (manual and hand piece) into the implant holder.
- CC/IC (No Holder): Fit the implant driver into the implant.
- Press to make a tight fit and raise the implant set slightly.
- EC/IC: Open the black cap on the bottom of the vial to remove the cover screw. CC/IC (No Holder): The cover screw is inside the coloured cap.

Information on the packaging

Implant box label

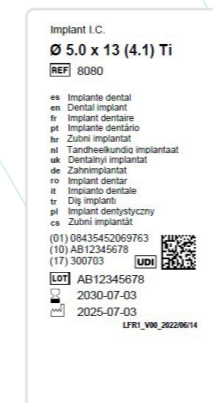


Labels that make the product traceable



Implant EC/IC/CC	External/internal/conical connection indicator
Ø 5.0 x 13 (4.1)	Diameter x length (platform)
Ti	Titanium
REF 8080	Reference number
LOT AB12345678	Batch code
YYMM-DD	Expiry date
STERILE R	Sterile. Sterilization method: radiation
ifu.avinent.com	Consult instructions for use
Manufacturer	Manufacturer
CE 0197	CE Mark NB num 0197. TÜV Rheinland
Rx only	(For the USA only) CAUTION: Federal law restricts this device to sale by or on the order of a physician
(01) 08435452001046 (10) AB12345678 (17) YYMMDD	UDI (Unique Device Identifier Carrier)
Do not re-use	Do not re-use
Do not re-sterilize	Do not re-sterilize
Do not use if package is damaged and consult instructions for use	Do not use if package is damaged and consult instructions for use
MD	Medical Device
Qty:1	Quantity of implants included in the packaging
Date of manufacture	Date of manufacture
Simple sterile barrier system with protective packaging inside	Simple sterile barrier system with protective packaging inside

Avinent Guided surgery

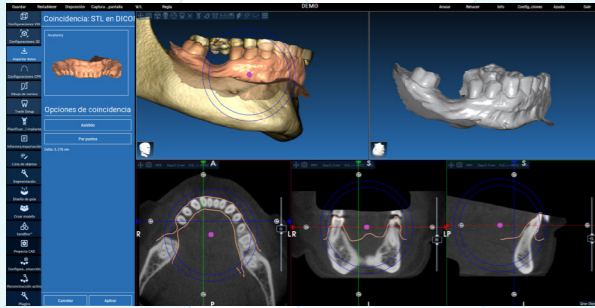

Avinent Guided Surgery

- Surgical Guide Box 3DIEMME®
- Implant planning software with Real Guide®

CT or CBCT Scanners. Available libraries for:

- NewTom
- Carestream
- (More coming soon)


Surgical motors

Avinent offers a wide range of surgical motors designed for many clinical applications, produced by leading brands in the industry. Intended to simplify daily practice and for multiple users, they can be adapted to suit each practitioner's needs by allowing the entire drilling sequence to be customised.

Our surgical motors are ergonomically designed, easy to use and significantly help to reduce tiredness. They give implantology specialists a surgical unit for everyday use in safely carrying out oral procedures. All the surgical motors have been designed with the aim of minimising size and weight, to improve the balance of the instrument and motor in the practitioner's hand and thereby reduce tiredness during long treatments.

Bien Air[®]
Dental

NSK

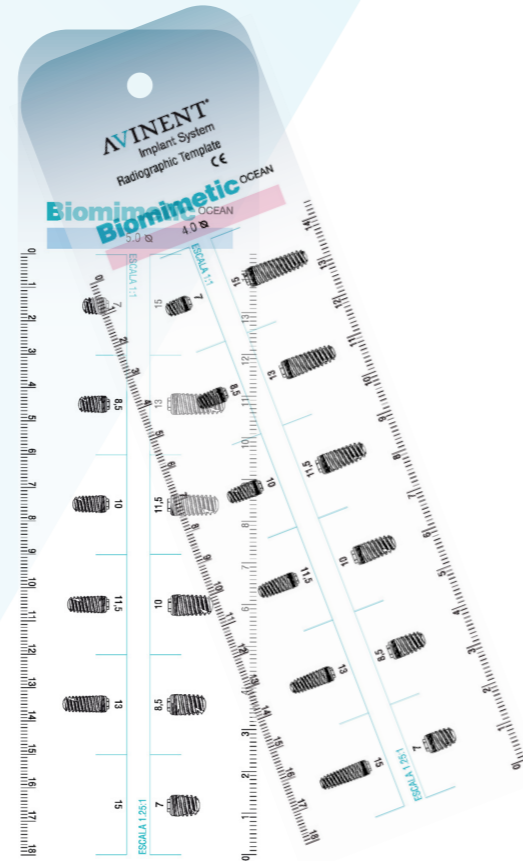

Radiographic template

The radiographic template is a guide to help practitioners precisely select the appropriate implant diameter and length. To adapt it to the proportions of the x-ray, the dimensions of the implant are shown at a scale 1:1 and 1.25:1.

Product index

REF.	DESCRIPTION	PAGE	REF.	DESCRIPTION	PAGE
0003	Healing abutment EC 4,1 x 5 x 5	4	0609	Aesthetic healing abutment IC 4,5 x 4	6
0030	Healing abutment EC 3,5 x 4 x 3	4	0610	Aesthetic healing abutment IC 4,5 x 5	6
0031	Healing abutment EC 3,5 x 4 x 4	4	0611	Aesthetic healing abutment IC 4,5 x 6	6
0032	Healing abutment EC 3,5 x 4 x 5	4	0612	Aesthetic healing abutment IC 4,5 x 7	6
0033	Healing abutment EC 3,5 x 5 x 3	4	0644	Screwdriver L18 (Hex 1.20)	10
0034	Healing abutment EC 3,5 x 5 x 4	4	0645	Screwdriver L30 (Hex 1.20)	10
0035	Healing abutment EC 3,5 x 5 x 5	4	0648	Screwdriver for Angled Transep. Abut. L30	10
0036	Healing abutment EC 4,1 x 5 x 3	4	0651	Holding tool EC/IC	10
0037	Healing abutment EC 4,1 x 5 x 4	4	KI589B204	Drill extension	10
0038	Healing abutment EC 4,1 x 5 x 7	4	0723	Screwdriver Impr. Coping Closed Tray L20.5	10
0171	Anatomic healing abutment EC 3,5 x 5 x 3	4	0726	Screwdriver for Transep. Abutment L30	10
0172	Anatomic healing abutment EC 3,5 x 5 x 4	4	0790	Handle ISO 1797 L	11
0173	Anatomic healing abutment EC 3,5 x 5 x 5	4	0791	Handle ISO 1797 S	11
0174	Anatomic healing abutment EC 4,1 x 5 x 3	4	0804	Screwdriver for Angled Transep. Abut. L25	10
0175	Anatomic healing abutment EC 4,1 x 5 x 4	4	1558	Implant EC 3,5 x 10 (3,5)	4
0176	Anatomic healing abutment EC 4,1 x 5 x 5	4	1559	Implant EC 3,5 x 11,5 (3,5)	4
0177	Anatomic healing abutment EC 4,1 x 5 x 7	4	1560	Implant EC 3,5 x 13 (3,5)	4
0188	Pointed drill	10	1561	Implant EC 3,5 x 15 (3,5)	4
0263	Screwdriver for Gold Screw/RHEIN83®	10	1562	Implant EC 4,0 x 7 (3,5)	4
0267	Screwdriver for Grooved Screw	10	1563	Implant EC 4,0 x 8,5 (3,5)	4
0274	Screwdriver S (048)	10	1564	Implant EC 4,0 x 10 (3,5)	4
0275	Screwdriver L (048)	10	1565	Implant EC 4,0 x 11,5 (3,5)	4
0277	Screwdriver L22 (Hex 1.20)	10	1566	Implant EC 4,0 x 13 (3,5)	4
0278	Implant driver S (2.5)	10	1567	Implant EC 4,0 x 15 (3,5)	4
0295	Torque wrench	10	1568	Implant EC 4,5 x 7 (4,1)	4
0299	Implant driver L (2.5)	10	1569	Implant EC 4,5 x 8,5 (4,1)	4
0300	Holder Driver EC/IC L22	10	1570	Implant EC 4,5 x 10 (4,1)	4
0328	Screwdriver for Transep. Abutment L22	10	1571	Implant EC 4,5 x 11,5 (4,1)	4
0465	Anatomic healing abutment IC 3,5/4,1 x 4,5 x 2	6	1572	Implant EC 4,5 x 13 (4,1)	4
0466	Anatomic healing abutment IC 3,5/4,1 x 4,5 x 3	6	1573	Implant EC 4,5 x 15 (4,1)	4
0467	Anatomic healing abutment IC 3,5/4,1 x 4,5 x 3	6	1574	Implant EC 5,0 x 7 (4,1)	4
0468	Anatomic healing abutment IC 3,5/4,1 x 4,5 x 5	6	1575	Implant EC 5,0 x 8,5 (4,1)	4
0469	Anatomic healing abutment IC 3,5/4,1 x 4,5 x 7	6	1576	Implant EC 5,0 x 10 (4,1)	4
0471	Anatomic healing abutment IC 3,5/4,1 x 5,5 x 3	6	1577	Implant EC 5,0 x 11,5 (4,1)	4
0472	Anatomic healing abutment IC 3,5/4,1 x 5,5 x 4	6	1578	Implant EC 5,0 x 13 (4,1)	4
0473	Anatomic healing abutment IC 3,5/4,1 x 5,5 x 5	6	8149	Implant IC 3,5 x 7 (3,5)	6
0474	Anatomic healing abutment IC 3,5/4,1 x 5,5 x 7	6	8150	Implant IC 3,5 x 8,5 (3,5)	6
0526	MiniBox	10	8147	Implant IC 3,5 x 7 (3,5) No Holder	7
0607	Aesthetic healing abutment IC 4,5 x 2	6	8148	Implant IC 3,5 x 8,5 (3,5) No Holder	7
0608	Aesthetic healing abutment IC 4,5 x 3	6	1579	Implant IC 3,5 x 10 (3,5)	6

REF.	DESCRIPTION	PAGE	REF.	DESCRIPTION	PAGE
1580	Implant IC 3,5 x 11,5 (3,5)	6	8144	Implant CC 3,5 x 8,5 (3,5)	8
1581	Implant IC 3,5 x 13 (3,5)	6	2935	Implant CC 3,5 x 10 (3,5)	8
1582	Implant IC 3,5 x 15 (3,5)	6	2936	Implant CC 3,5 x 11,5 (3,5)	8
1583	Implant IC 4,0 x 7 (3,5)	6	2937	Implant CC 3,5 x 13 (3,5)	8
1584	Implant IC 4,0 x 8,5 (3,5)	6	2938	Implant CC 3,5 x 15 (3,5)	8
1585	Implant IC 4,0 x 10 (3,5)	6	2939	Implant CC 4,0 x 7 (3,5)	8
1586	Implant IC 4,0 x 11,5 (3,5)	6	2940	Implant CC 4,0 x 8,5 (3,5)	8
1587	Implant IC 4,0 x 13 (3,5)	6	2941	Implant CC 4,0 x 10 (3,5)	8
1588	Implant IC 4,0 x 15 (3,5)	6	2942	Implant CC 4,0 x 11,5 (3,5)	8
1589	Implant IC 4,5 x 7 (4,1)	6	2943	Implant CC 4,0 x 13 (3,5)	8
1590	Implant IC 4,5 x 8,5 (4,1)	6	2944	Implant CC 4,0 x 15 (3,5)	8
1591	Implant IC 4,5 x 10 (4,1)	6	2945	Implant CC 4,5 x 7 (4,1)	8
1592	Implant IC 4,5 x 11,5 (4,1)	6	2946	Implant CC 4,5 x 8,5 (4,1)	8
1593	Implant IC 4,5 x 13 (4,1)	6	2947	Implant CC 4,5 x 10 (4,1)	8
1594	Implant IC 4,5 x 15 (4,1)	6	2948	Implant CC 4,5 x 11,5 (4,1)	8
1595	Implant IC 5,0 x 7 (4,1)	6	2949	Implant CC 4,5 x 13 (4,1)	8
1596	Implant IC 5,0 x 8,5 (4,1)	6	2950	Implant CC 4,5 x 15 (4,1)	8
1597	Implant IC 5,0 x 10 (4,1)	6	2951	Implant CC 5,0 x 7 (4,1)	8
1598	Implant IC 5,0 x 11,5 (4,1)	6	2952	Implant CC 5,0 x 8,5 (4,1)	8
1599	Implant IC 5,0 x 13 (4,1)	6	2953	Implant CC 5,0 x 10 (4,1)	8
1763	Sterilization cassette OCEAN	10	2954	Implant CC 5,0 x 11,5 (4,1)	8
1810	Direction indicator ø 1,5 - ø 2,3	11	2955	Implant CC 5,0 x 13 (4,1)	8
1878	Implant handle S	11	2981	Implant Driver CC 3.5 & CC.I 3.5 (Short)	10
2046	Twist drill ø 1,6 x 7 - 15	11	2982	Implant Driver CC 4.1 & CC.I 4.1 (Short)	10
2047	Pilot drill ø 1,6 - ø 2,4	11	2984	Implant Driver CC 3.5 & CC.I 3.5 (Long)	10
2048	Drill ø 2,0 - ø 3,3 x 7 - 15	11	2985	Implant Driver CC 4.1 & CC.I 4.1 (Long)	10
2049	Drill ø 2,2 - ø 3,8 x 7 - 15	11	2988	Anatomic healing abutment (Single) CC 3,5 x 4 x 3	8
2050	Drill ø 2,8 - ø 4,3 x 7 - 15	11	2989	Anatomic healing abutment (Single) CC 3,5 x 4 x 5	8
2051	Drill ø 3,2 - ø 4,8 x 7 - 13	11	2990	Anatomic healing abutment (Single) CC 3,5 x 5 x 3	8
2687	Screw tap 3,5 mm	11	2991	Anatomic healing abutment (Single) CC 3,5 x 5 x 5	8
2688	Screw tap 4,0 mm	11	2992	Anatomic healing abutment (Single) CC 3,5 x 5 x 7	8
2689	Screw tap 4,5 mm	11	2993	Anatomic healing abutment (Multiple) CC 3,5 x 4 x 3	8
2690	Screw tap 5,0 mm	11	2994	Anatomic healing abutment (Multiple) CC 3,5 x 4 x 5	8
2692	Holder Driver WH EC/IC L22	10	2995	Anatomic healing abutment (Multiple) CC 3,5 x 5 x 3	8
2693	Holder Driver EC/IC L18	10	2996	Anatomic healing abutment (Multiple) CC 3,5 x 5 x 5	8
2726	Anatomic healing abutment IC 3,5/4,1 x 6,5 x 5	6	2997	Anatomic healing abutment (Multiple) CC 3,5 x 5 x 7	8
2727	Anatomic healing abutment IC 3,5/4,1 x 6,5 x 4	6	2998	Anatomic healing abutment (Single) CC 4,1 x 5 x 3	8
2737	Anatomic healing abutment IC 3,5/4,1 x 6,5 x 3	6	2999	Anatomic healing abutment (Single) CC 4,1 x 5 x 5	8
2891	Implant handle L	11	3000	Anatomic healing abutment (Single) CC 4,1 x 5 x 7	8
8143	Implant CC 3,5 x 7 (3,5)	8	3008	Anatomic healing abutment (Multiple) CC 4,1 x 5 x 7	8

REF.	DESCRIPTION	PAGE	REF.	DESCRIPTION	PAGE
3010	Anatomic healing abutment (Multiple) CC 4,1 x 6 x 3	8	6986	Drill Stop Ø1.3-2.4 L10	12
3011	Anatomic healing abutment (Multiple) CC 4,1 x 6 x 5	8	6987	Drill Stop Ø1.3-2.4 L11.5	12
3012	Anatomic healing abutment (Multiple) CC 4,1 x 6 x 7	8	6988	Drill Stop Ø1.3-2.4 L13	12
3311	Hard bone drill ø 2,4 - ø 3,3 x 7 - 15	11	6989	Drill Stop Ø1.3-2.4 L15	12
3312	Hard bone drill ø 3,0 - ø 3,7 x 7 - 15	11	6990	CORAL/OCEAN/ICEBERG Drill Stop Ø2.8-3.3 L7	12
3313	Hard bone drill ø 3,8 - ø 4,3 x 7 - 15	11	6991	CORAL/OCEAN/ICEBERG Drill Stop Ø2.8-3.3 L8.5	12
3314	Hard bone drill ø 4,1 - ø 4,7 x 7 - 13	11	6992	CORAL/OCEAN/ICEBERG Drill Stop Ø2.8-3.3 L10	12
3363	Healing abutment EC 4,5 x 4 x 3	4	6993	CORAL/OCEAN/ICEBERG Drill Stop Ø2.8-3.3 L11.5	12
3364	Healing abutment EC 4,5 x 4 x 5	4	6994	CORAL/OCEAN/ICEBERG Drill Stop Ø2.8-3.3 L13	12
3365	Healing abutment EC 4,5 x 4 x 7	4	6995	CORAL/OCEAN/ICEBERG Drill Stop Ø2.8-3.3 L15	12
3370	Anatomic healing abutment IC 3,5/4,1 x 3,5 x 3	6	6996	CORAL/OCEAN/ICEBERG Drill Stop Ø3.2-3.8 L7	12
3371	Anatomic healing abutment IC 3,5/4,1 x 3,5 x 5	6	6997	CORAL/OCEAN/ICEBERG Drill Stop Ø3.2-3.8 L8.5	12
3372	Anatomic healing abutment IC 3,5/4,1 x 3,5 x 7	6	6998	CORAL/OCEAN/ICEBERG Drill Stop Ø3.2-3.8 L10	12
3470	Anatomic healing abutment (Single) CC 4,1 x 6 x 3	8	6999	CORAL/OCEAN/ICEBERG Drill Stop Ø3.2-3.8 L11.5	12
3471	Anatomic healing abutment (Single) CC 4,1 x 6 x 5	8	7000	CORAL/OCEAN/ICEBERG Drill Stop Ø3.2-3.8 L13	12
3472	Anatomic healing abutment (Single) CC 4,1 x 6 x 7	8	7001	CORAL/OCEAN/ICEBERG Drill Stop Ø3.2-3.8 L15	12
3473	Anatomic healing abutment (Multiple) CC 4,1 x 5 x 3	8	7002	CORAL/OCEAN/ICEBERG Drill Stop Ø3.6-4.3 L7	12
3474	Anatomic healing abutment (Multiple) CC 4,1 x 5 x 5	8	7003	CORAL/OCEAN/ICEBERG Drill Stop Ø3.6-4.3 L8.5	12
3812	Implant CC 6,0 x 7 (4,1)	8	7004	CORAL/OCEAN/ICEBERG Drill Stop Ø3.6-4.3 L10	12
3814	Implant CC 6,0 x 11,5 (4,1)	8	7005	CORAL/OCEAN/ICEBERG Drill Stop Ø3.6-4.3 L11.5	12
3938	Implant CC 6,0 x 8,5 (4,1)	8	7006	CORAL/OCEAN/ICEBERG Drill Stop Ø3.6-4.3 L13	12
3939	Implant CC 6,0 x 10 (4,1)	8	7007	CORAL/OCEAN/ICEBERG Drill Stop Ø3.6-4.3 L15	12
3960	Hard bone drill ø 5,1 - ø 5,7 x 7 - 11,5	11	7008	CORAL/OCEAN/ICEBERG Drill Stop Ø4.2-4.8 L7	12
3963	Screw tap 6,0 mm	11	7009	CORAL/OCEAN/ICEBERG Drill Stop Ø4.2-4.8 L8.5	12
6344	Implant CC 4,5 x 7,0 (3,5)	10	7010	CORAL/OCEAN/ICEBERG Drill Stop Ø4.2-4.8 L10	12
6345	Implant CC 4,5 x 8,5 (3,5)	10	7011	CORAL/OCEAN/ICEBERG Drill Stop Ø4.2-4.8 L11.5	12
6346	Implant CC 4,5 x 10,0 (3,5)	10	7012	CORAL/OCEAN/ICEBERG Drill Stop Ø4.2-4.8 L13	12
6347	Implant CC 4,5 x 11,5 (3,5)	10	7013	OCEAN Drill Stop Ø5.7 L7	12
6348	Implant CC 4,5 x 13,0 (3,5)	10	7014	OCEAN Drill Stop Ø5.7 L8.5	12
6349	Implant CC 4,5 x 15,0 (3,5)	10	7015	OCEAN Drill Stop Ø5.7 L10	12
6350	Implant CC 5,0 x 7,0 (3,5)	10	7016	OCEAN Drill Stop Ø5.7 L11.5	12
6351	Implant CC 5,0 x 8,5 (3,5)	10	7959	Drill Stop Kit for implants up to Ø4.5	12
6352	Implant CC 5,0 x 10,0 (3,5)	10	7960	Drill Stop Set for implants from Ø4.8 to Ø6.0	12
6353	Implant CC 5,0 x 11,5 (3,5)	10	8032	OCEAN/ICEBERG Twist Drill Ø2.0-3.3 L7-15	11
6354	Implant CC 5,0 x 13,0 (3,5)	10	8033	OCEAN/ICEBERG Twist Drill Ø2.2-3.8 L7-15	11
6984	Drill Stop Ø1.3-2.4 L7	12	8034	OCEAN/ICEBERG Twist Drill Ø2.8-4.3 L7-15	11
6985	Drill Stop Ø1.3-2.4 L8.5	12	8035	OCEAN/ICEBERG Twist Drill Ø3.2-4.8 L7-13	11

*The availability of the products in this catalog may vary depending on the country where you are based. Please contact your Avinent distributor for further information.

REF.	DESCRIPTION	PAGE
8036	OCEAN Twist Drill Ø4.2-5.7 L7-11.5	11
8037	OCEAN/ICEBERG Twist Drill Ø2.4-3.3 L7-15	11
8038	OCEAN/ICEBERG Twist Drill Ø3.0-3.7 L7-15	11
8039	OCEAN/ICEBERG Twist Drill Ø3.8-4.3 L7-15	11
8040	OCEAN/ICEBERG Twist Drill Ø4.1-4.7 L7-13	11
8041	OCEAN Twist Drill Ø5.1-5.7 L7-11.5	11
8060	Implant IC 3.5 Ø3.5 L10 (No Holder)	8
8061	Implant IC 3.5 Ø3.5 L11.5 (No Holder)	8
8062	Implant IC 3.5 Ø3.5 L13 (No Holder)	8
8063	Implant IC 3.5 Ø3.5 L15 (No Holder)	8
8064	Implant IC 3.5 Ø4.0 L7 (No Holder)	8
8065	Implant IC 3.5 Ø4.0 L8.5 (No Holder)	8
8066	Implant IC 3.5 Ø4.0 L10 (No Holder)	8
8067	Implant IC 3.5 Ø4.0 L11.5 (No Holder)	8
8068	Implant IC 3.5 Ø4.0 L13 (No Holder)	8
8069	Implant IC 3.5 Ø4.0 L15 (No Holder)	8
8070	Implant IC 4.1 Ø4.5 L7 (No Holder)	8
8071	Implant IC 4.1 Ø4.5 L8.5 (No Holder)	8
8072	Implant IC 4.1 Ø4.5 L10 (No Holder)	8
8073	Implant IC 4.1 Ø4.5 L11.5 (No Holder)	8
8074	Implant IC 4.1 Ø4.5 L13 (No Holder)	8
8075	Implant IC 4.1 Ø4.5 L15 (No Holder)	8
8076	Implant IC 4.1 Ø5.0 L7 (No Holder)	8
8077	Implant IC 4.1 Ø5.0 L8.5 (No Holder)	8
8078	Implant IC 4.1 Ø5.0 L10 (No Holder)	8
8079	Implant IC 4.1 Ø5.0 L11.5 (No Holder)	8
8080	Implant IC 4.1 Ø5.0 L13 (No Holder)	8
8082	Implant Driver IC 3.5/4.1 (Short)	12
8083	Implant Driver IC 3.5/4.1 (Long)	12



Carretera de Navarcles, 107
Pol. Industrial Santa Anna I
08251 Santpedor (Barcelona) - España
T. (+34) 93 827 34 65
www.avinent.com - avinent@avinent.com

AVINENT AUSTRALIA
australia@avinent.com

AVINENT BENELUX
benelux@avinent.com

AVINENT CANADA
canada@avinent.com

AVINENT COLOMBIA
colombia@avinent.com

AVINENT CROATIA
croatia@avinent.com

AVINENT FRANCE
france@avinent.com

AVINENT KUWAIT
kuwait@avinent.com

AVINENT LITHUANIA
lithuania@avinent.com

AVINENT POLAND
poland@avinent.com

AVINENT PORTUGAL
portugal@avinent.com

AVINENT ROMANIA
romania@avinent.com

AVINENT TAIWAN
taiwan@avinent.com

AVINENT UKRAINE
ukraine@avinent.com

AVINENT UNITED ARAB EMIRATES
uae@avinent.com

AVINENT UNITED KINGDOM
uk@avinent.com

AVINENT USA
usa@avinent.com

AVINENT VIETNAM
vietnam@avinent.com

AVINENT SAUDI ARABIA
ksa@avinent.com



Management
System
ISO 13485:2016
www.tuv.com

